
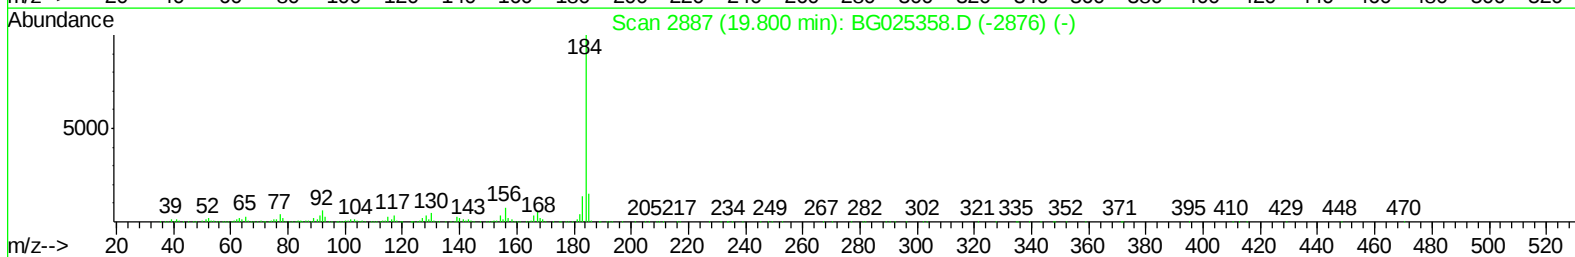
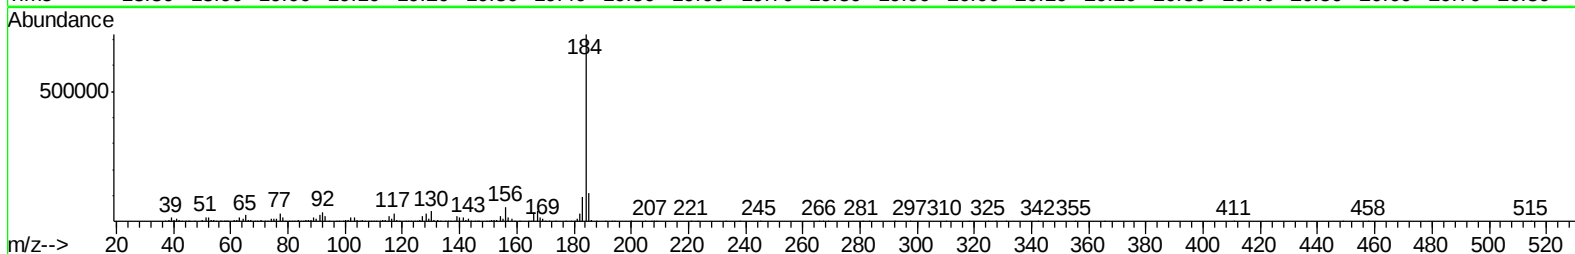


Data Path : Z:\HPCHEM1\BNA G\Data\BG123016\
Data File : BG025412.D
Acq On : 30 Dec 2016 13:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 04:04:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 18:42:01 2016
Response via : Initial Calibration

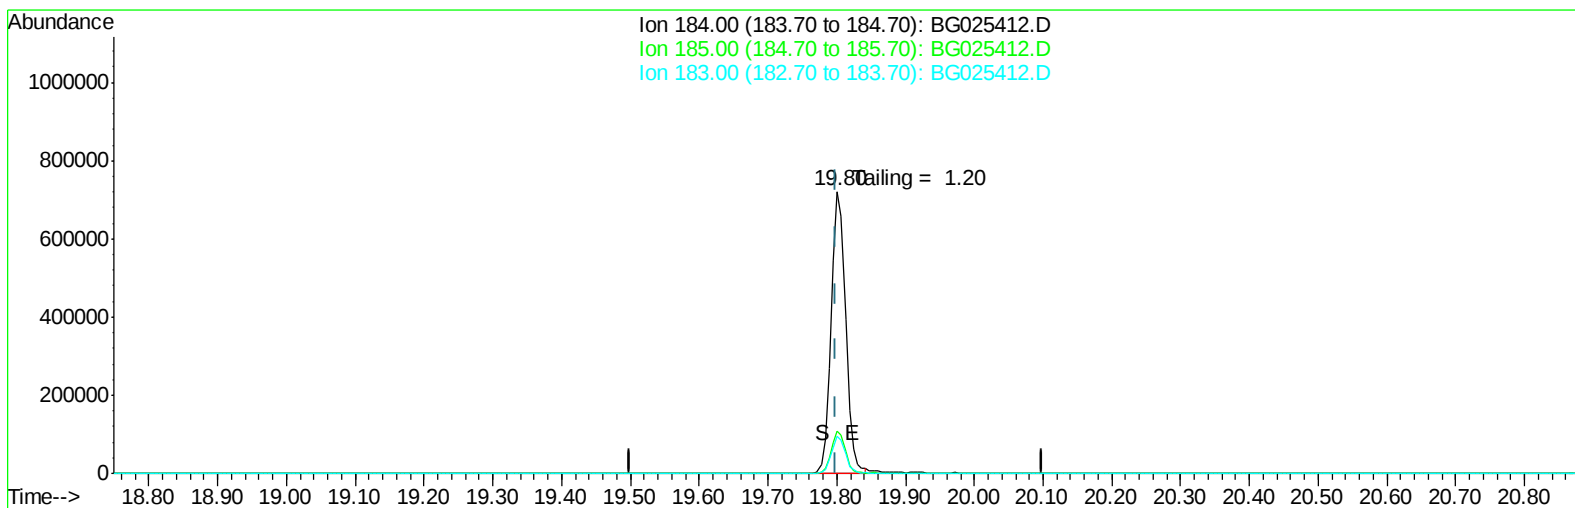

TIC: BG025412.D

(76) Benzidine




19.801min (+0.001) 613841.14ng

response 1056529

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.87
183.00	13.80	13.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG123016\
Data File : BG025412.D
Acq On : 30 Dec 2016 13:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 04:04:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 18:42:01 2016
Response via : Initial Calibration

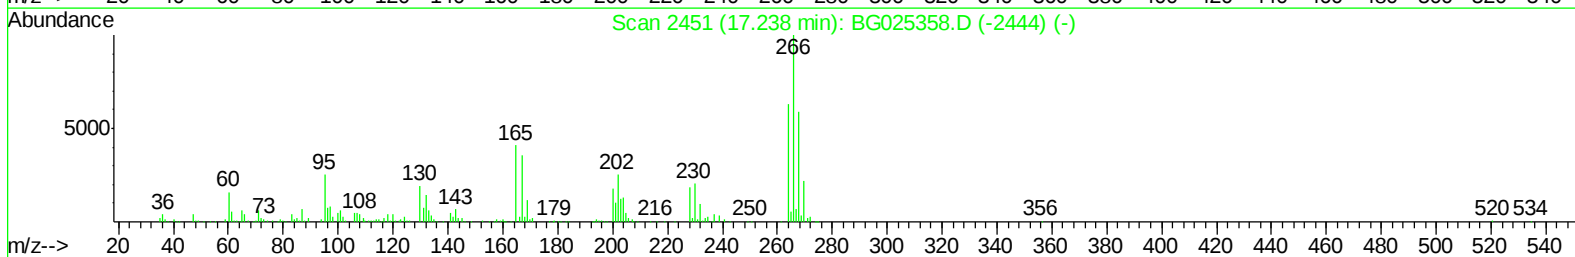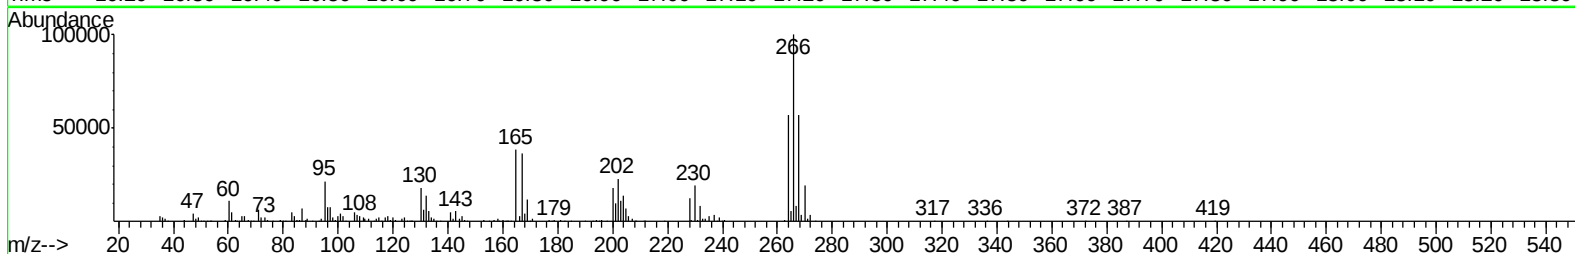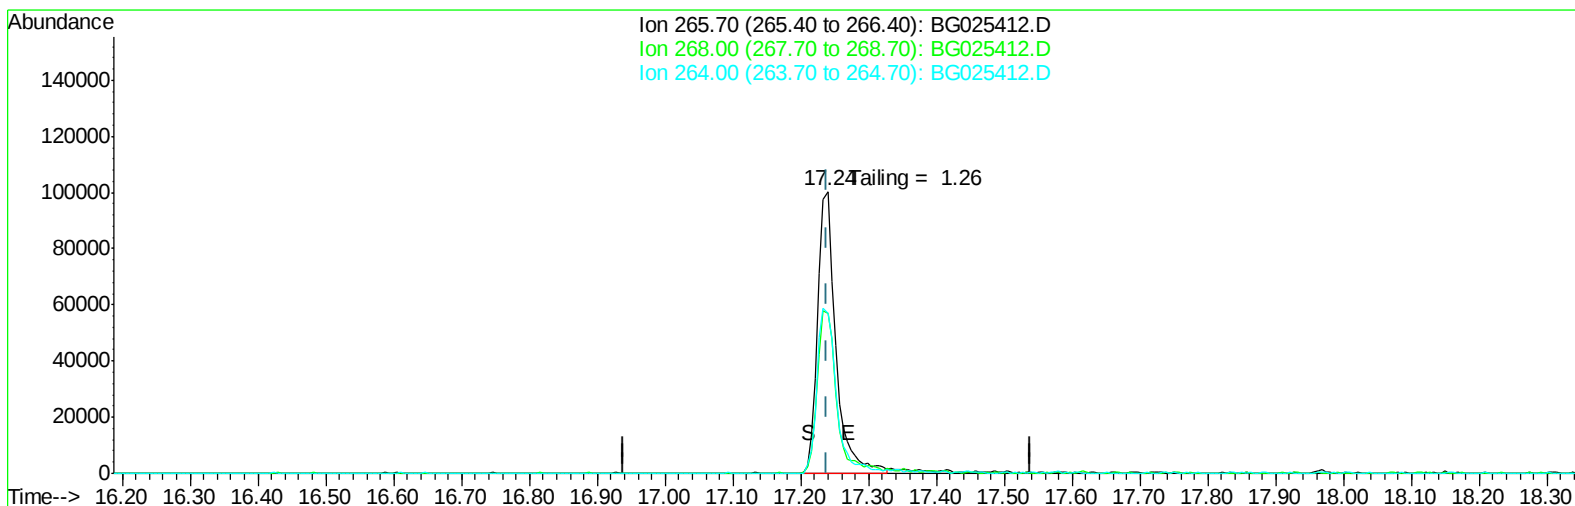

TIC: BG025412.D

(69) Pentachlorophenol (C)

17.239min (+0.001) 367462.36ng

response 186087

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	56.83
264.00	62.60	56.72
0.00	0.00	0.00