


Data Path : Z:\HPCHEM1\BNA G\Data\BG123016\
 Data File : BG025412.D
 Acq On : 30 Dec 2016 13:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

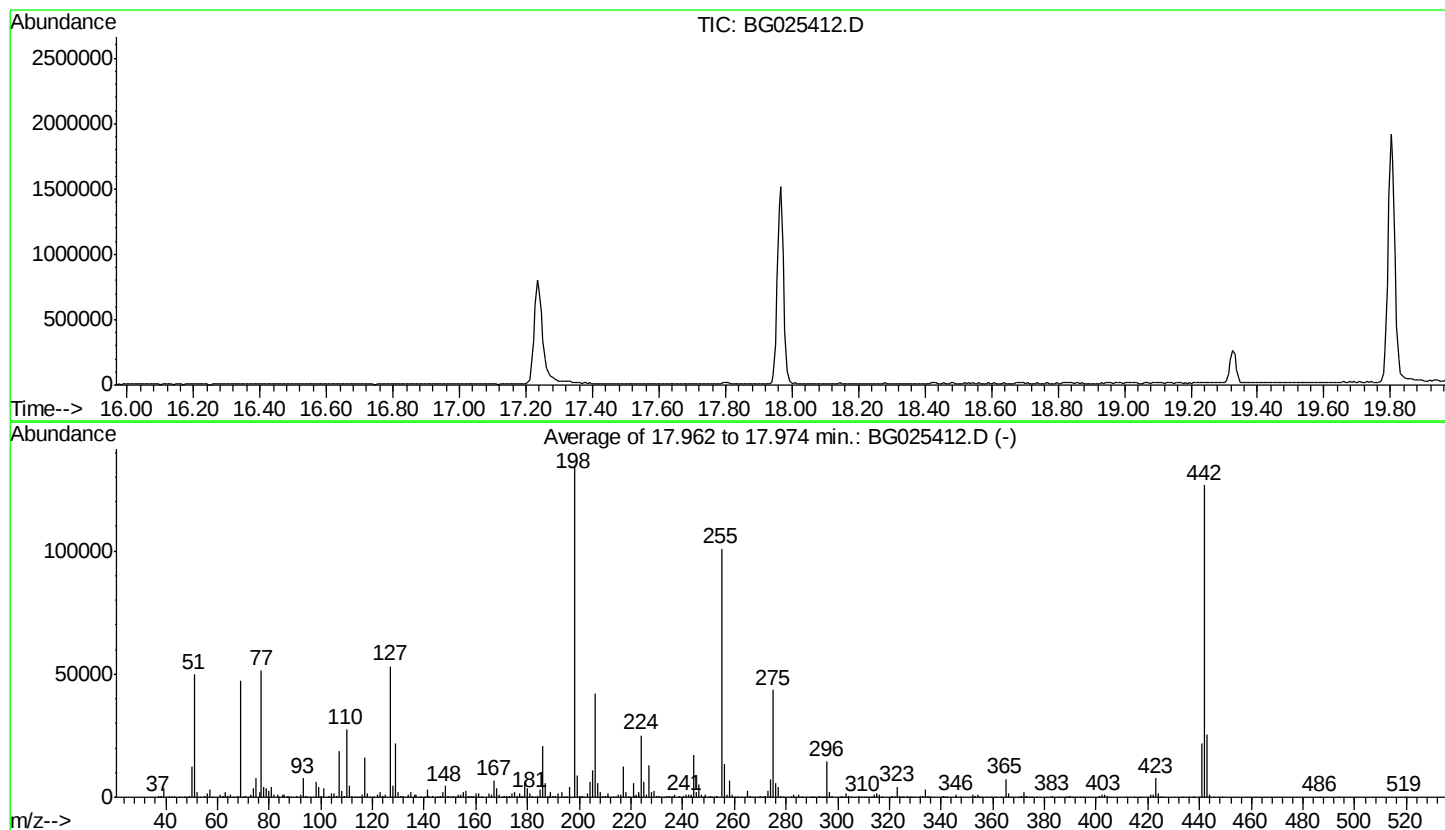

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	49698	PASS
68	69	0.00	2	1.2	564	PASS
69	198	0.00	100	35.2	47412	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	39.5	53149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134597	PASS
199	198	5	9	6.7	9009	PASS
275	198	10	60	32.4	43552	PASS
365	198	1	100	5.5	7442	PASS
441	442	0.01	24	17.1	21717	PASS
442	198	50	100	94.2	126746	PASS
443	442	15	24	20.1	25530	PASS