
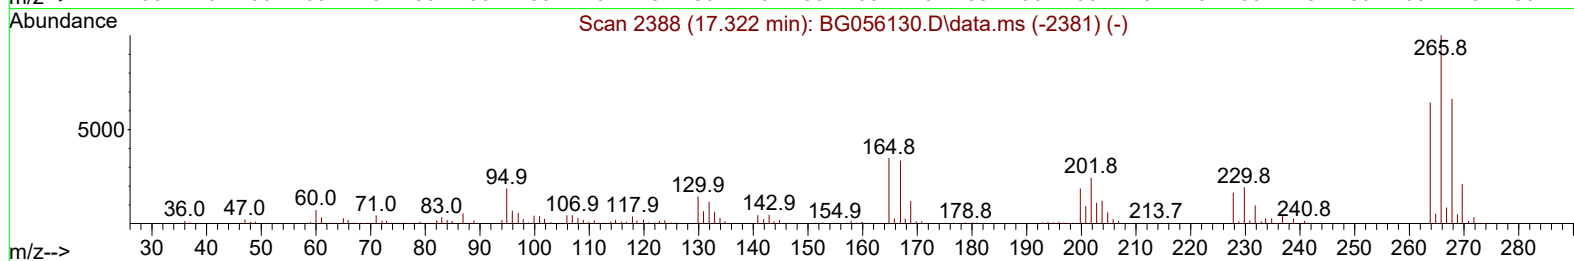
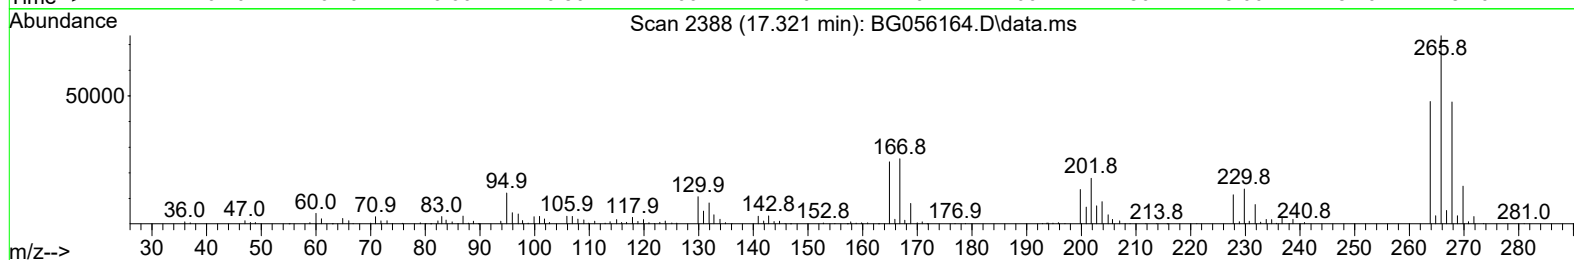


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123022\
Data File : BG056164.D
Acq On : 30 Dec 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 01:13:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

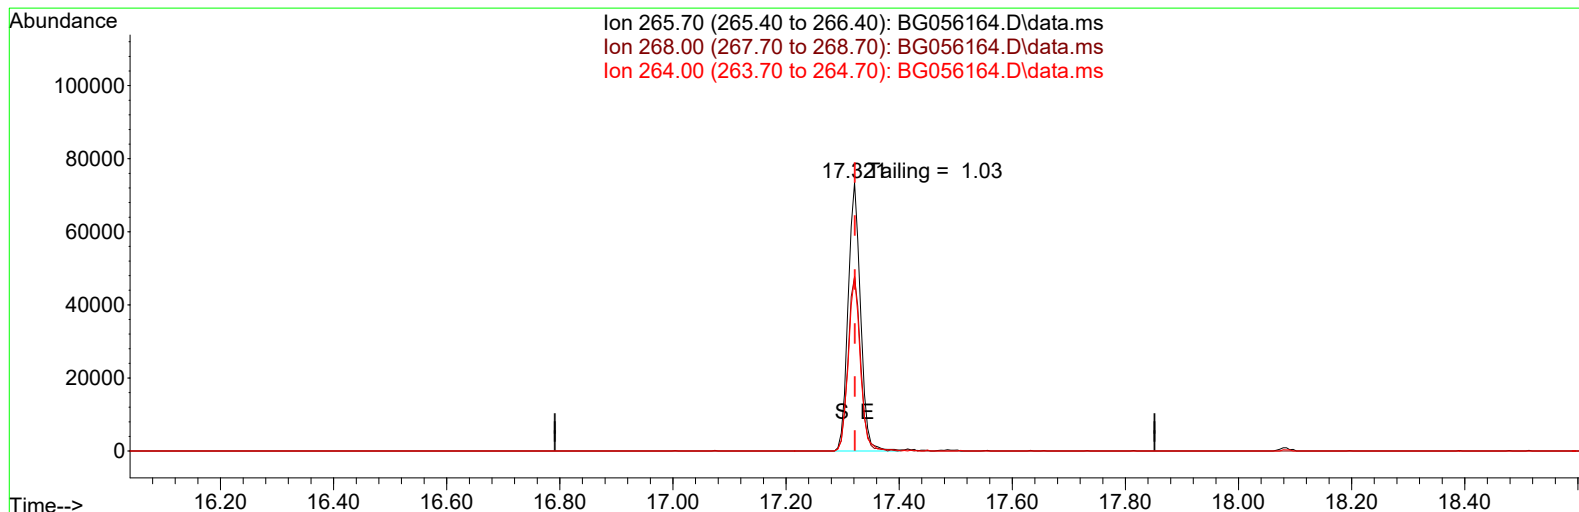

TIC: BG056164.D\data.ms

(70) Pentachlorophenol (C)




17.321min (-0.001) 9546.80 ng

response 112219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	64.82
264.00	64.30	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123022\
Data File : BG056164.D
Acq On : 30 Dec 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 01:13:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

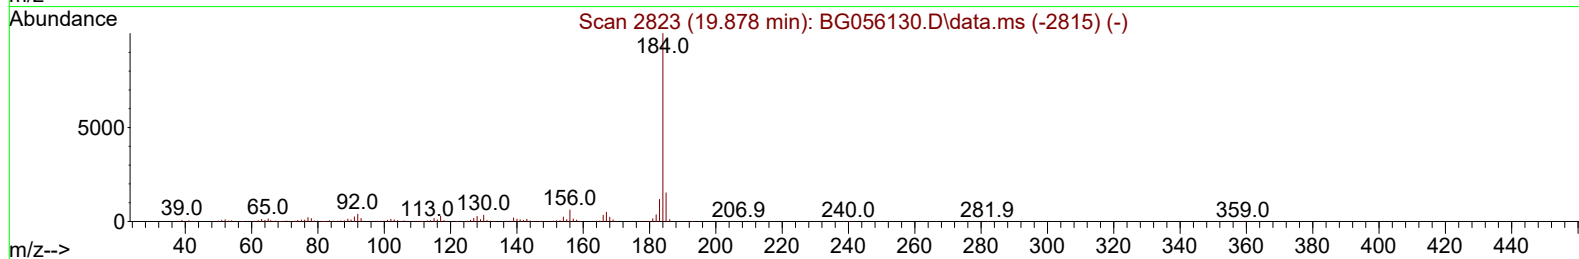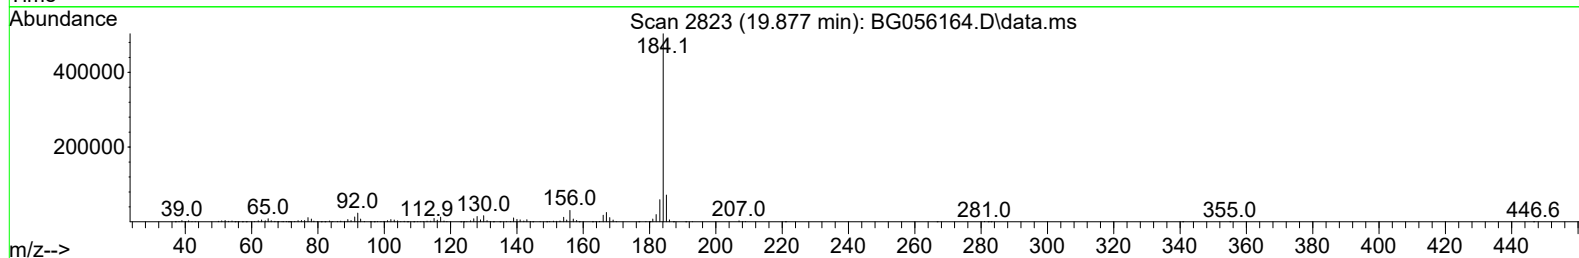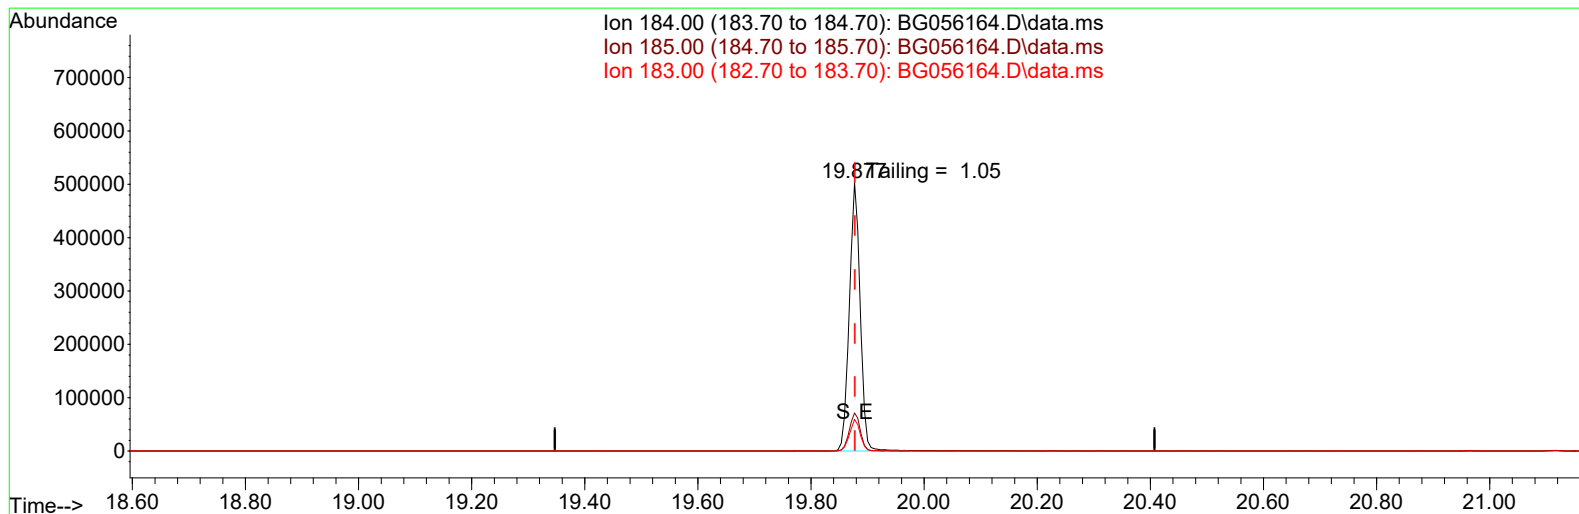

TIC: BG056164.D\data.ms

(77) Benzidine**19.877min (-0.001) 115021.03 ng****response 673149**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.20
183.00	11.70	11.79
0.00	0.00	0.00