
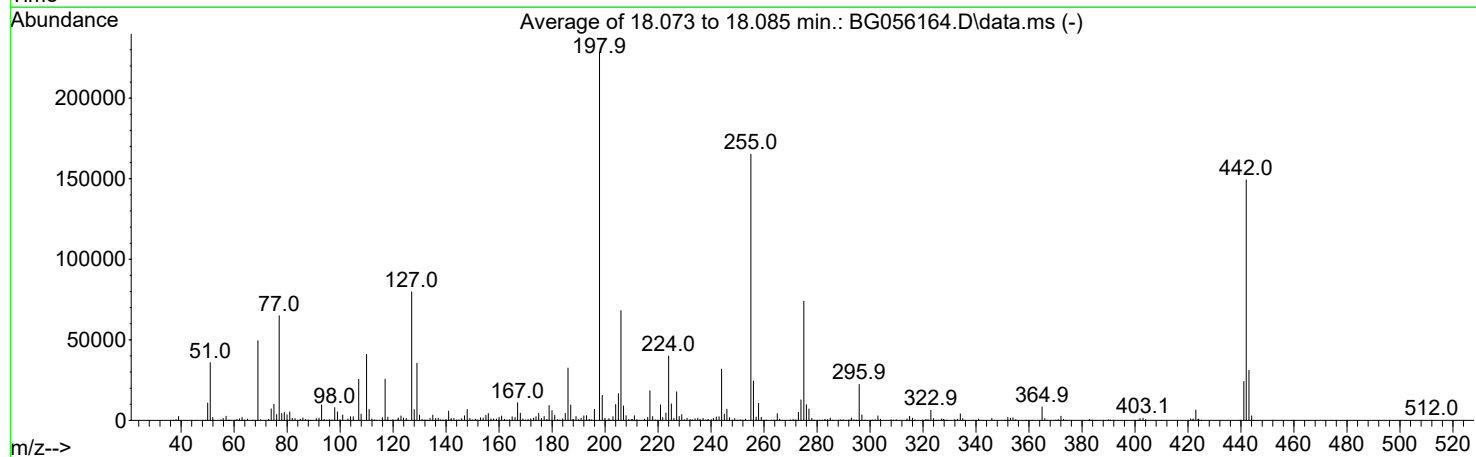


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123022\
Data File : BG056164.D
Acq On : 30 Dec 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 28 05:20:14 2022

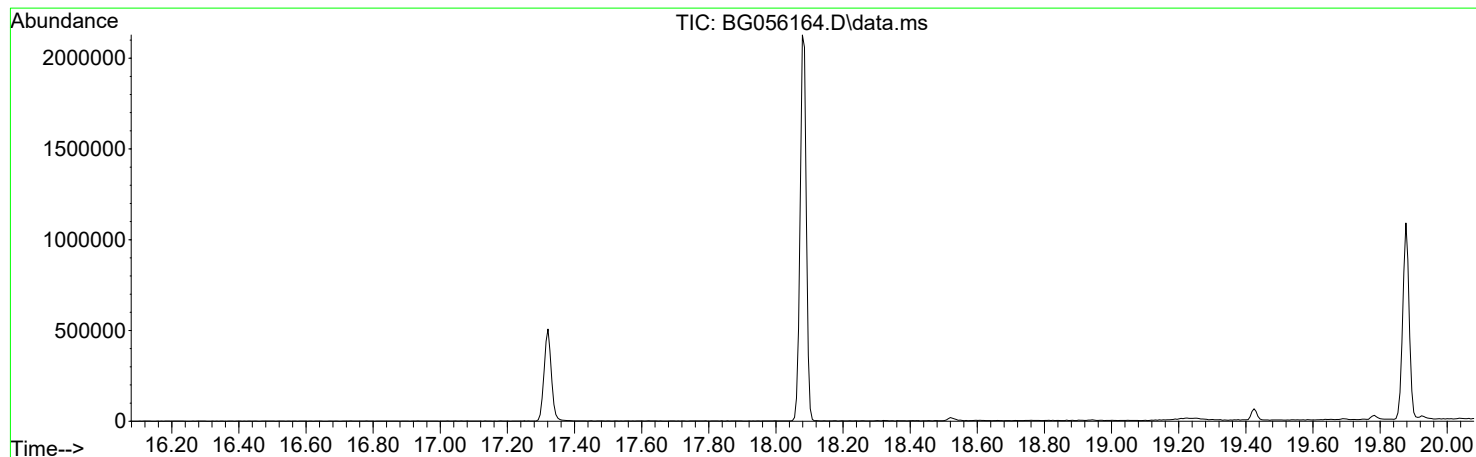

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.7	35835	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.7	49472	PASS
70	69	0.00	2	0.9	438	PASS
127	198	10	80	34.9	79768	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	228352	PASS
199	198	5	9	6.8	15535	PASS
275	198	10	60	32.4	74016	PASS
365	198	1	100	3.7	8391	PASS
441	198	0.01	100	10.6	24188	PASS
442	442	50	100	100.0	149315	PASS
443	442	15	24	20.8	31083	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2022	BNA_G	BG056164.D
Compound Name	Response	Retention Time
DDT	347864	21.116
DDD	7044	20.711
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7044	354908	1.98

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123022\
Data File : BG056164.D
Acq On : 30 Dec 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 31 01:13:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

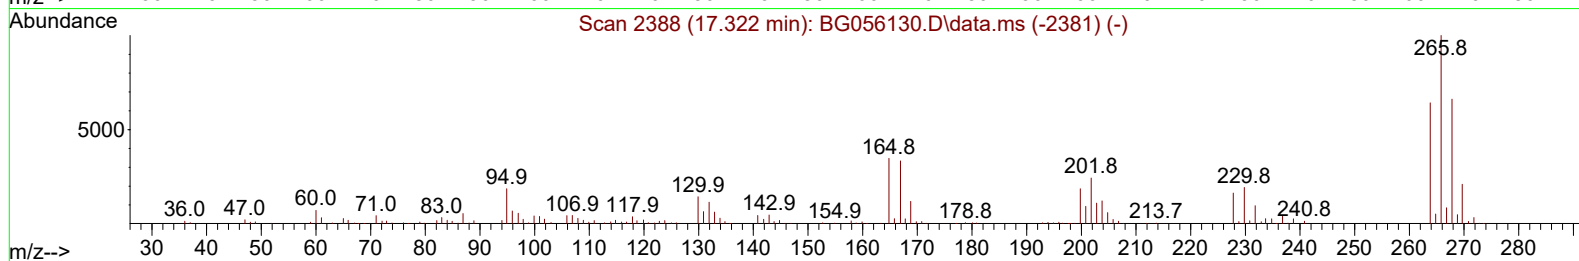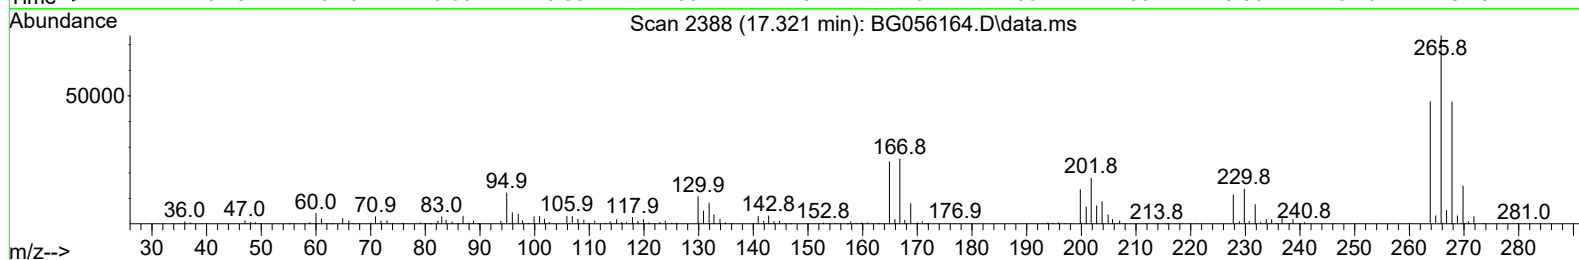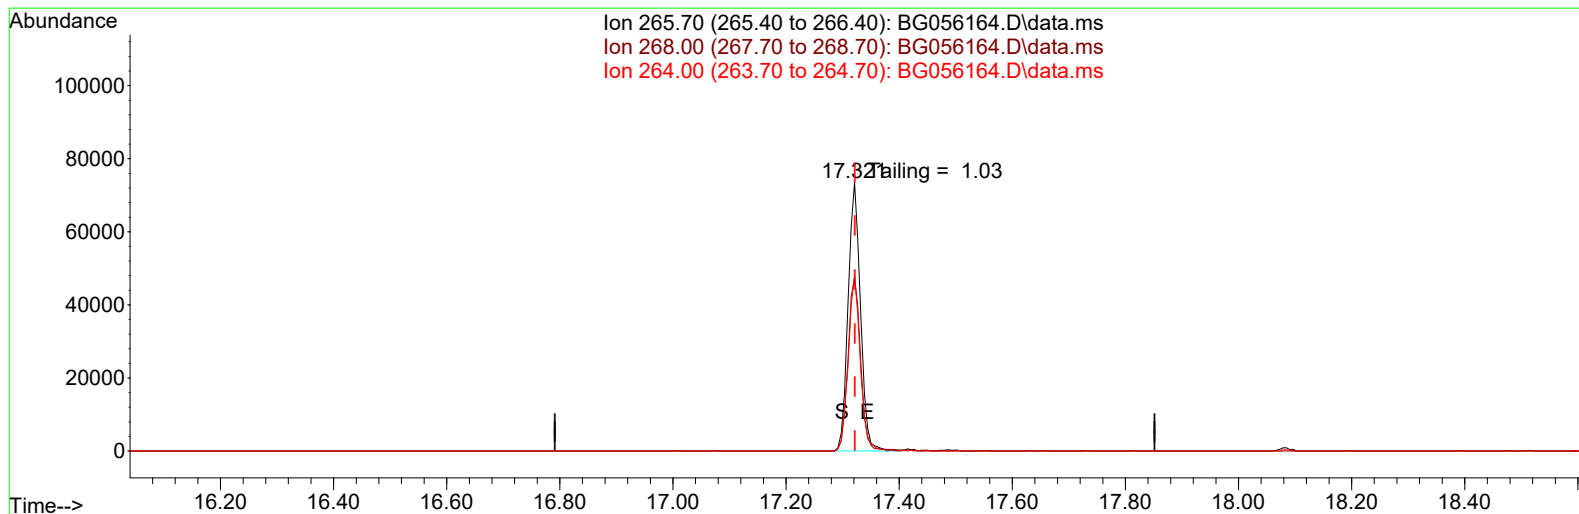

TIC: BG056164.D\data.ms

(70) Pentachlorophenol (C)

17.321min (-0.001) 9546.80 ng




response 112219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	64.82
264.00	64.30	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123022\
Data File : BG056164.D
Acq On : 30 Dec 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 31 01:13:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

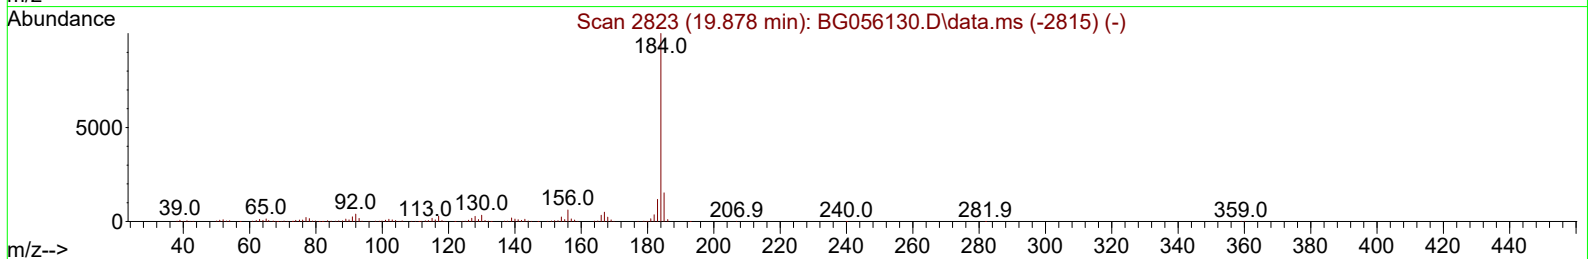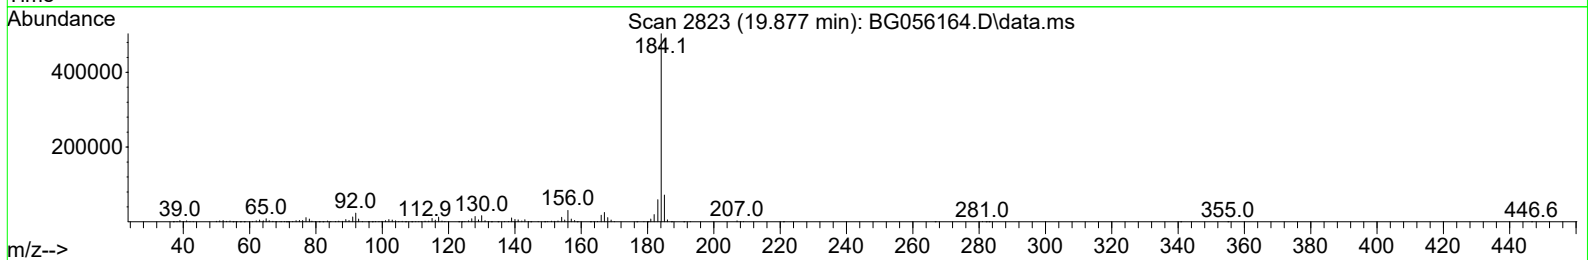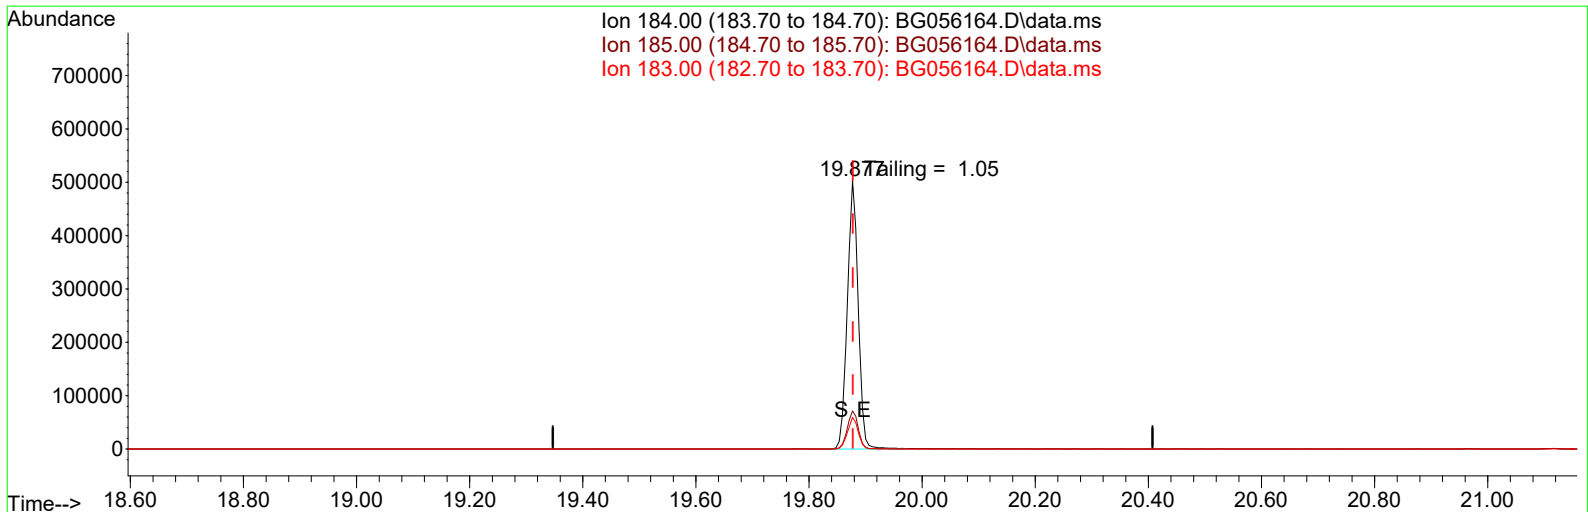

TIC: BG056164.D\data.ms

(77) Benzidine

19.877min (-0.001) 115021.03 ng

response 673149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.20
183.00	11.70	11.79
0.00	0.00	0.00