


Data Path : Z:\HPCHEM1\BNA_G\Data\BG123114\
Data File : BG015831.D
Acq On : 31 Dec 2014 18:20
Operator : TP/IZ
Sample : DFTPP98
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG123114.M
Title : SVOA CALIBRATION
Last Update : Thu Jan 01 00:49:59 2015

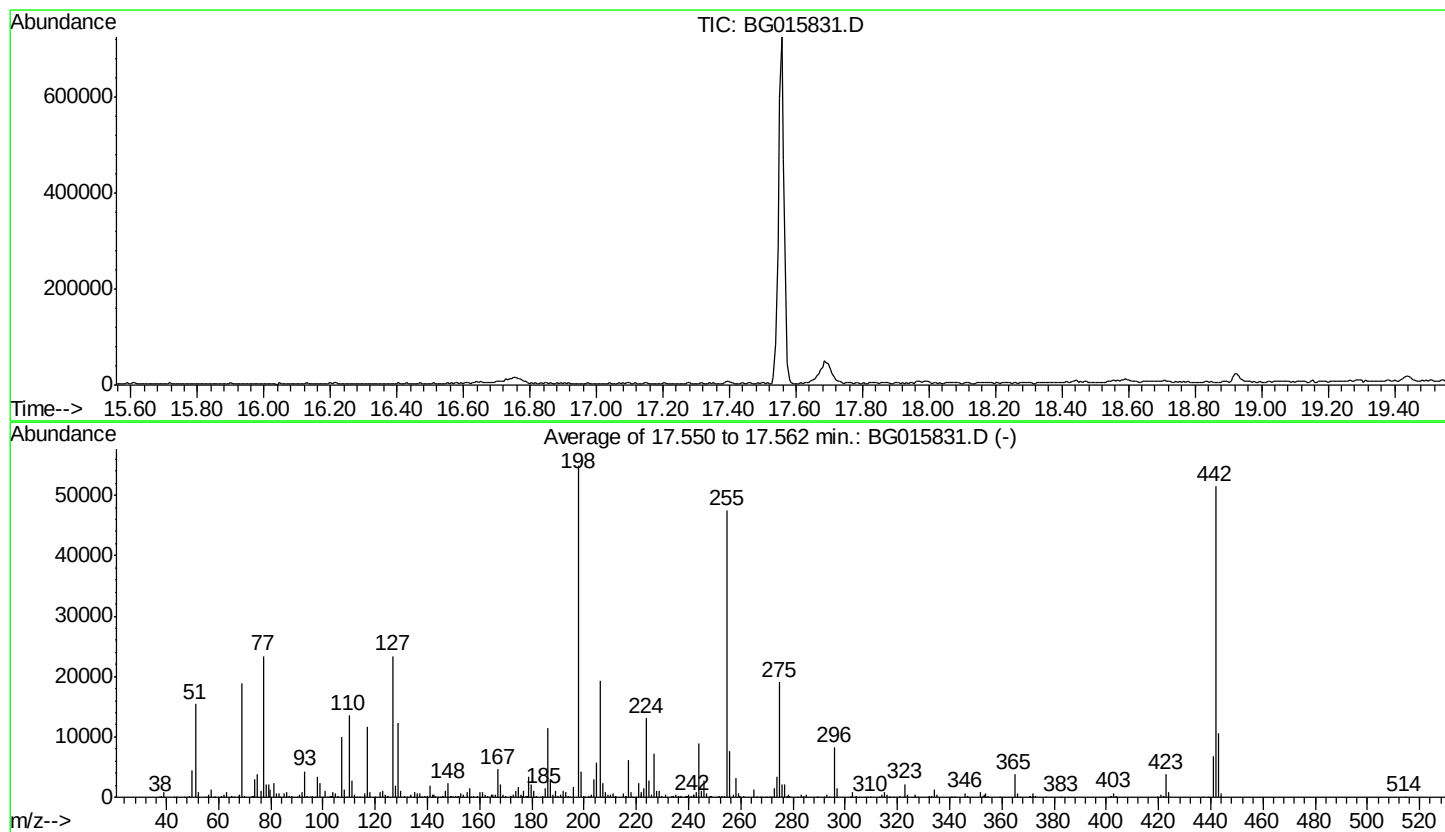

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	15437	PASS
68	69	0.00	2	1.9	366	PASS
69	198	0.00	100	34.3	18842	PASS
70	69	0.00	2	0.8	146	PASS
127	198	10	80	42.6	23368	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54914	PASS
199	198	5	9	7.6	4153	PASS
275	198	10	60	34.7	19033	PASS
365	198	1	100	6.8	3748	PASS
441	443	0.01	100	64.3	6768	PASS
442	198	50	100	93.7	51474	PASS
443	442	15	24	20.4	10524	PASS