

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
 Data File : BG020641.D
 Acq On : 31 Dec 2015 14:38
 Operator : UM/SJ
 Sample : PB87463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Quant Time: Jan 01 03:19:00 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 01 03:15:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	16020	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	67277	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.70	164	49833	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.44	188	126891	20.00	ng/ul	0.00
78) Chrysene-d12	21.72	240	157144	20.00	ng/ul	0.00
86) Perylene-d12	24.97	264	148529	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	2490	9.31	ng/uL	0.00
5) Phenol-d5	7.22	99	51790	38.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.38	67	32355	39.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.59	132	42151	40.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.77	113	45003	38.76	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	21374	41.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	25355	42.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	46372	40.46	ng/ul	0.00
29) 4-Chloroaniline-d4	11.01	131	63133	46.40	ng/ul	0.00
44) Dimethylphthalate-d6	14.10	166	173701	42.59	ng/ul	0.00
47) Acenaphthylene-d8	14.39	160	193450	41.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	22773	35.61	ng/ul	0.00
58) Fluorene-d10	15.69	176	153395	41.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	25602	33.27	ng/ul	0.00
71) Anthracene-d10	17.54	188	255140	43.16	ng/ul	0.00
79) Pyrene-d10	19.82	212	304520	43.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	333127	44.95	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.77	70	973	1.01	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
Data File : BG020641.D
Acq On : 31 Dec 2015 14:38
Operator : UM/SJ
Sample : PB87463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Quant Time: Jan 01 03:19:00 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 01 03:15:46 2016
Response via : Initial Calibration

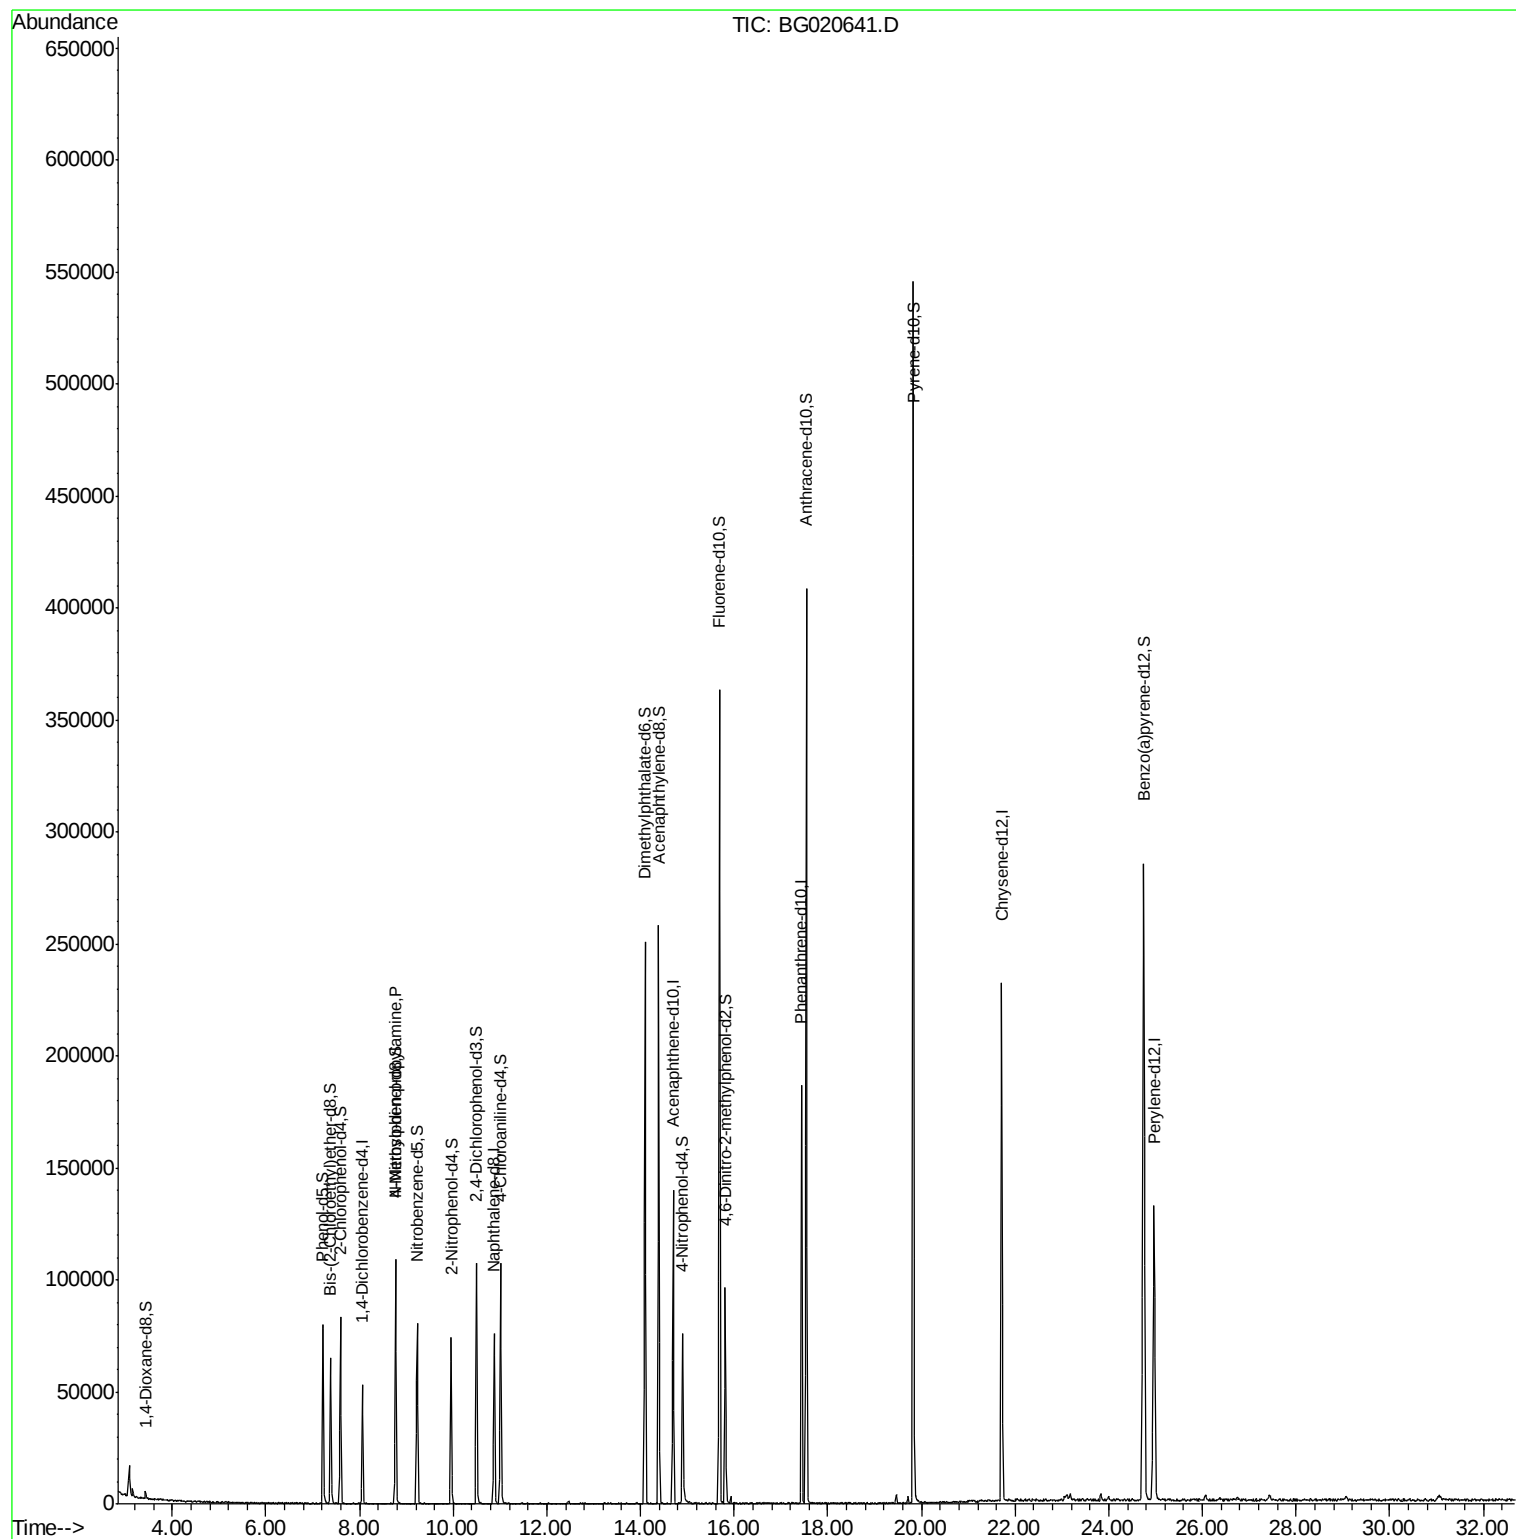

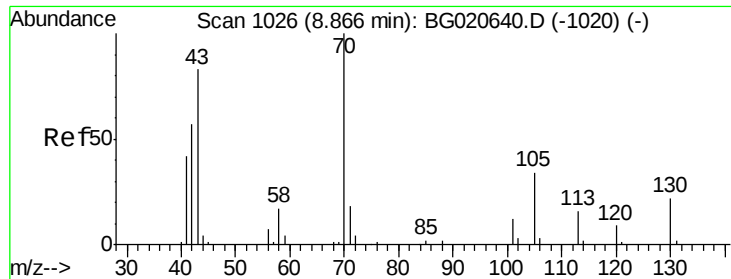

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 8.77 min Scan# 1009
 Delta R.T. -0.10 min
 Lab File: BG020641.D
 Acq: 31 Dec 2015 14:38

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Tgt Ion: 70 Resp: 973
 Ion Ratio Lower Upper
 70 100
 42 365.9 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

