

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
 Data File : BG020641.D
 Acq On : 31 Dec 2015 14:38
 Operator : UM/SJ
 Sample : PB87463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.079	34	41	51	rVV3	13677	29529	3.77%	0.445%
2	3.156	51	54	60	rVB3	4212	6388	0.81%	0.096%
3	3.432	97	101	109	rVB3	3762	6024	0.77%	0.091%
4	3.679	140	143	146	rVB3	630	948	0.12%	0.014%
5	3.714	146	149	152	rBV4	824	1048	0.13%	0.016%
6	4.061	203	208	210	rVB2	901	1232	0.16%	0.019%
7	4.196	228	231	234	rBV2	695	1024	0.13%	0.015%
8	7.216	739	745	753	rBV	80221	141387	18.03%	2.133%
9	7.380	766	773	785	rBV	65052	108821	13.88%	1.642%
10	7.592	802	809	820	rBB	83377	144330	18.41%	2.177%
11	8.062	881	889	899	rBB	53211	89050	11.36%	1.343%
12	8.767	1003	1009	1020	rBV	109175	189614	24.18%	2.861%
13	9.231	1080	1088	1100	rBV	80744	146163	18.64%	2.205%
14	9.954	1205	1211	1219	rBV	74486	129664	16.54%	1.956%
15	10.494	1297	1303	1315	rBV	107509	196804	25.10%	2.969%
16	10.876	1361	1368	1376	rBV	76085	135782	17.32%	2.048%
17	11.011	1385	1391	1402	rBV	107280	193912	24.73%	2.925%
18	12.457	1634	1637	1642	rBB2	999	1706	0.22%	0.026%
19	14.096	1910	1916	1924	rBV	250977	353109	45.04%	5.327%
20	14.390	1959	1966	1974	rBV	258205	398983	50.89%	6.019%
21	14.695	2010	2018	2026	rBB3	140200	220671	28.15%	3.329%
22	14.895	2047	2052	2067	rBV	75831	137619	17.55%	2.076%
23	15.688	2180	2187	2195	rBV	363567	540362	68.92%	8.152%
24	15.753	2195	2198	2200	rVB	928	882	0.11%	0.013%
25	15.812	2203	2208	2218	rVV	96589	139075	17.74%	2.098%
26	15.929	2223	2228	2233	rBV2	3238	4393	0.56%	0.066%
27	17.233	2446	2450	2453	rVB	812	1210	0.15%	0.018%
28	17.439	2479	2485	2493	rBV	186768	289425	36.92%	4.366%
29	17.539	2496	2502	2512	rVB	408490	616120	78.58%	9.295%
30	19.466	2823	2830	2834	rBV	4116	6554	0.84%	0.099%
31	19.713	2868	2872	2876	rVB	3350	4309	0.55%	0.065%
32	19.825	2884	2891	2903	rBV	545297	779634	99.44%	11.762%
33	19.901	2903	2904	2908	rVV2	1089	1436	0.18%	0.022%
34	20.071	2930	2933	2936	rBV2	556	818	0.10%	0.012%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
 Data File : BG020641.D
 Acq On : 31 Dec 2015 14:38
 Operator : UM/SJ
 Sample : PB87463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Title : SVOA CALIBRATION

35	21.240	3128	3132	3134	rBV	1015	1020	0.13%	0.015%
36	21.464	3168	3170	3175	rVB3	949	1060	0.14%	0.016%
37	21.716	3205	3213	3224	rBV	231490	387009	49.36%	5.839%
38	21.828	3228	3232	3236	rVB2	532	985	0.13%	0.015%
39	21.869	3236	3239	3243	rBV3	684	1086	0.14%	0.016%
40	22.151	3284	3287	3291	rVB3	786	967	0.12%	0.015%
41	22.304	3310	3313	3316	rVB3	848	980	0.12%	0.015%
42	22.369	3321	3324	3326	rBV2	925	810	0.10%	0.012%
43	22.451	3335	3338	3341	rBV2	838	954	0.12%	0.014%
44	22.715	3380	3383	3385	rVB2	768	808	0.10%	0.012%
45	23.021	3433	3435	3437	rBV2	1357	1467	0.19%	0.022%
46	23.097	3445	3448	3449	rBV2	1446	1623	0.21%	0.024%
47	23.179	3457	3462	3464	rVB5	2108	2592	0.33%	0.039%
48	23.614	3534	3536	3541	rVB2	756	1040	0.13%	0.016%
49	23.667	3541	3545	3548	rVB3	926	1303	0.17%	0.020%
50	23.773	3559	3563	3564	rVB3	1028	1241	0.16%	0.019%
51	23.785	3564	3565	3568	rBV3	1119	861	0.11%	0.013%
52	23.826	3568	3572	3579	rBV3	3379	6767	0.86%	0.102%
53	23.990	3592	3600	3607	rBV6	2045	5158	0.66%	0.078%
54	24.155	3624	3628	3629	rBV2	918	795	0.10%	0.012%
55	24.490	3683	3685	3686	rBV	864	791	0.10%	0.012%
56	24.525	3689	3691	3697	rVB2	776	1435	0.18%	0.022%
57	24.595	3701	3703	3706	rBV3	749	1084	0.14%	0.016%
58	24.748	3718	3729	3742	rBV	284212	784029	100.00%	11.828%
59	24.854	3745	3747	3751	rVV2	627	795	0.10%	0.012%
60	24.971	3753	3767	3777	rBV2	131516	362146	46.19%	5.464%
61	25.042	3777	3779	3782	rVB2	1147	1140	0.15%	0.017%
62	25.618	3873	3877	3879	rVB2	767	859	0.11%	0.013%
63	25.671	3883	3886	3891	rBV3	695	1138	0.15%	0.017%
64	26.058	3946	3952	3953	rBV4	2278	3210	0.41%	0.048%
65	26.340	3998	4000	4002	rBV2	1059	805	0.10%	0.012%
66	26.370	4002	4005	4007	rVB4	1032	1019	0.13%	0.015%
67	26.658	4050	4054	4058	rBV5	744	1255	0.16%	0.019%
68	27.151	4134	4138	4139	rVB2	1033	963	0.12%	0.015%
69	27.181	4139	4143	4146	rBV2	748	927	0.12%	0.014%
70	27.398	4178	4180	4182	rBV2	1215	1390	0.18%	0.021%
71	27.421	4182	4184	4187	rVV3	1268	1650	0.21%	0.025%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
 Data File : BG020641.D
 Acq On : 31 Dec 2015 14:38
 Operator : UM/SJ
 Sample : PB87463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Title : SVOA CALIBRATION

72	27.645	4216	4222	4225	rBV3	774	1448	0.18%	0.022%
73	27.739	4235	4238	4242	rBV4	703	1108	0.14%	0.017%
74	27.933	4270	4271	4276	rVB3	777	1024	0.13%	0.015%
75	28.438	4355	4357	4360	rVB2	892	863	0.11%	0.013%
76	28.644	4390	4392	4395	rVB2	939	1053	0.13%	0.016%
77	28.714	4403	4404	4408	rVB2	1044	956	0.12%	0.014%
78	29.055	4459	4462	4463	rVV	809	812	0.10%	0.012%
79	29.149	4474	4478	4480	rBV3	692	853	0.11%	0.013%
80	29.196	4485	4486	4490	rVB2	1041	1104	0.14%	0.017%
81	29.225	4490	4491	4494	rBV2	670	859	0.11%	0.013%
82	29.255	4494	4496	4500	rVB3	832	1223	0.16%	0.018%
83	29.443	4526	4528	4530	rVB	940	790	0.10%	0.012%
84	29.748	4576	4580	4583	rVB2	805	1111	0.14%	0.017%
85	30.142	4644	4647	4649	rVB2	637	818	0.10%	0.012%
86	30.189	4651	4655	4658	rBV3	1117	1376	0.18%	0.021%
87	30.330	4678	4679	4684	rVB3	716	978	0.12%	0.015%
88	30.394	4684	4690	4691	rBV	678	1004	0.13%	0.015%
89	30.765	4751	4753	4757	rVB2	943	859	0.11%	0.013%
90	31.000	4789	4793	4795	rBV3	1100	1820	0.23%	0.027%
91	31.035	4795	4799	4800	rVV4	1493	1468	0.19%	0.022%
92	31.064	4802	4804	4806	rVB3	1038	815	0.10%	0.012%
93	31.605	4892	4896	4899	rVB4	739	971	0.12%	0.015%
94	31.852	4935	4938	4941	rBV4	611	829	0.11%	0.013%
95	32.075	4973	4976	4980	rBV2	552	1014	0.13%	0.015%
96	32.516	5048	5051	5052	rBV2	816	858	0.11%	0.013%
97	32.604	5064	5066	5071	rBV3	818	1191	0.15%	0.018%


Sum of corrected areas: 6628393

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG123115\
Data File : BG020641.D
Acq On : 31 Dec 2015 14:38
Operator : UM/SJ
Sample : PB87463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

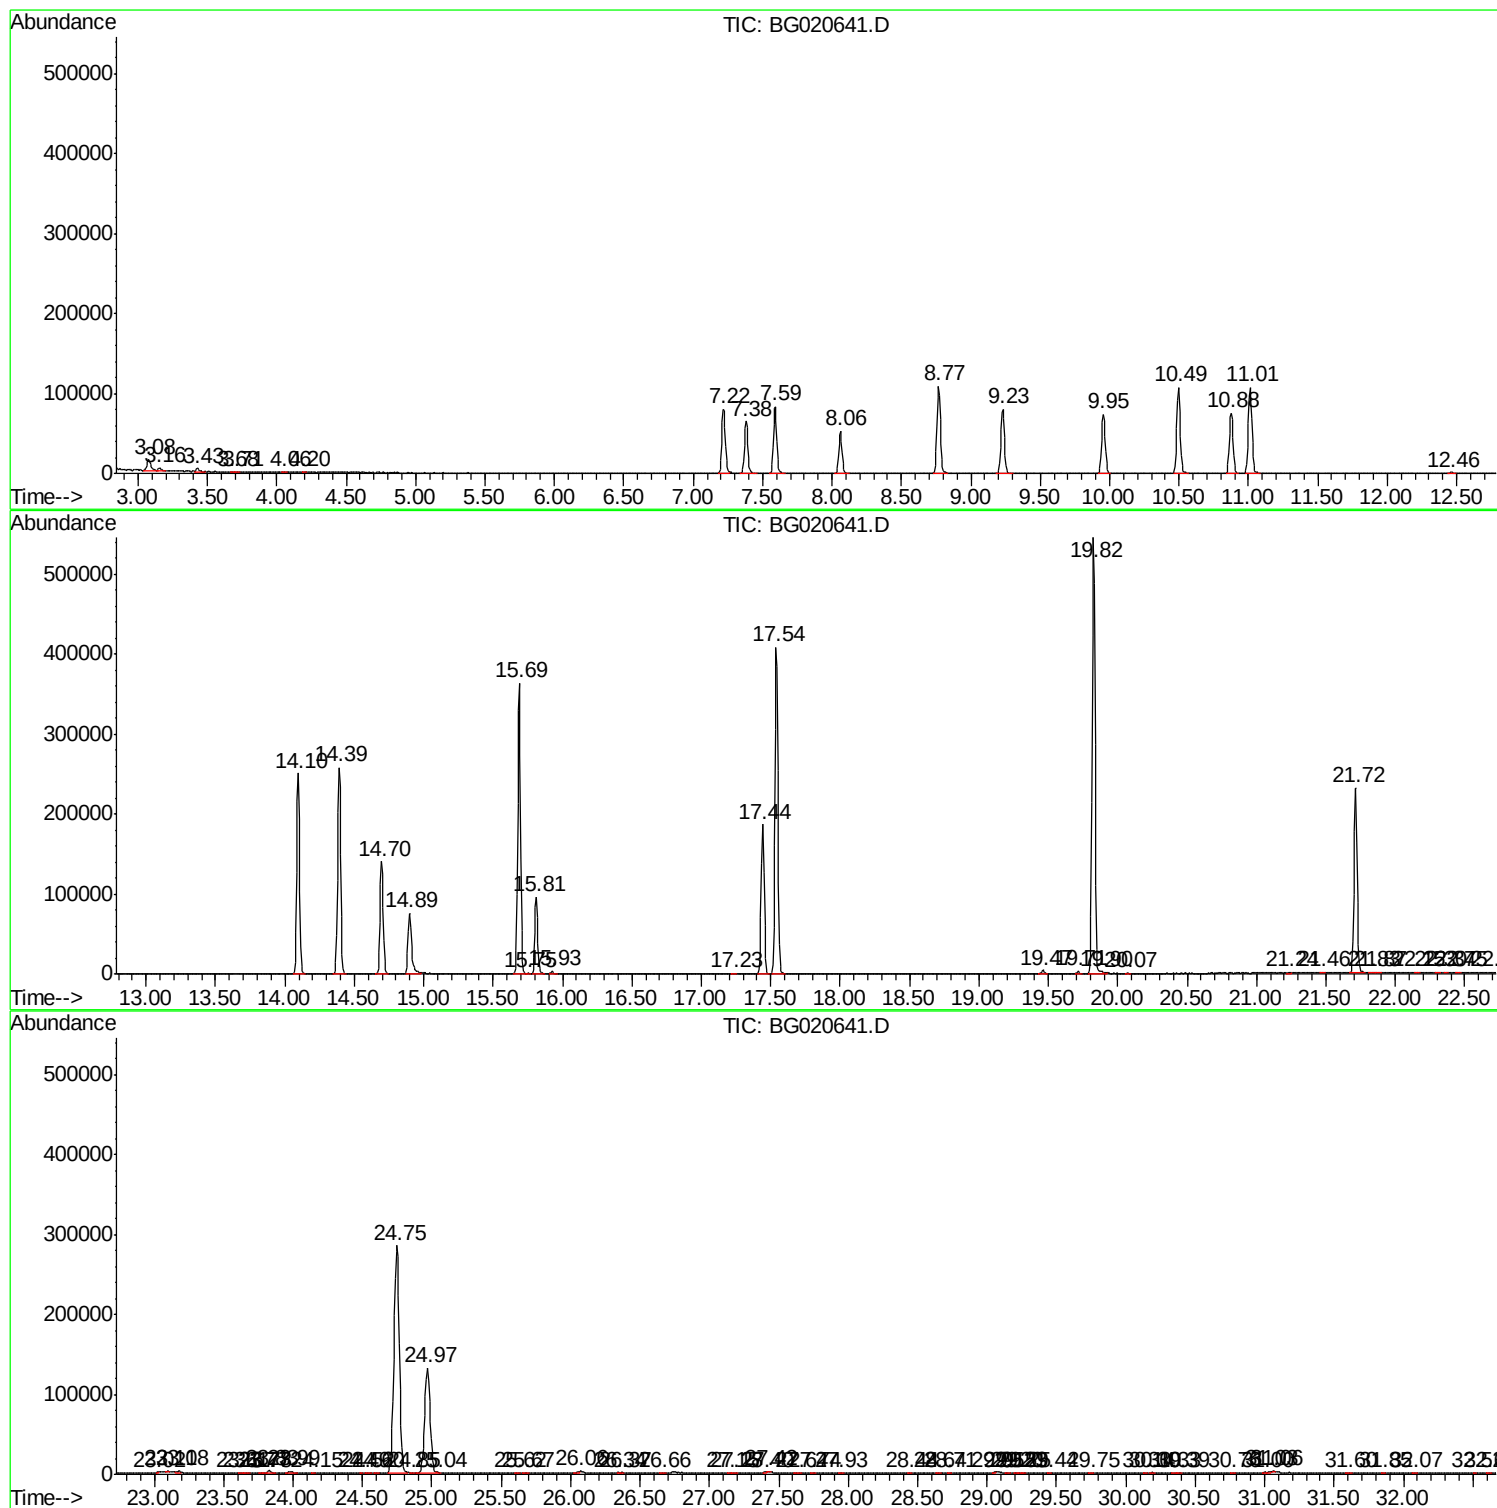

DbaaaPath::ZZ\NRPBMM1BBAAGCDBAAABBG23155\
 DbaaaFile::BB0000011DD
 AcqQOn ::331Dec2005 144388
 Operator::UMMSJ
 Sample::PBB8706BBL
 Misc:::
 ASSVal::33 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

QcandMebdd::ZZ\NRPBMM1BBAAGCMEH00SS0000222EPABBG230055MM
 QcandTitle::SUACALIBRATION

TICLibrary::CC\DATA\BASSENDS\02LL
 TICIntegratIonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
