

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB011013\HB001045.D Vial: 12
Acq On : 11-Jan-2013, 03:20 Operator: QM
Sample : E1002-01RE Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jan 11 12:14 2013 Quant Results File: HB011013.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB011013.M
Title :
Last Update : Fri Jan 11 12:05:05 2013
Response via : Initial Calibration
DataAcq Meth : NEWTEST.M

Volume Inj. : 50 ul
Signal Phase : Synergi HYDRO-RP
Signal Info : 250 X 4.60 mm 4 micron

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds


Target Compounds


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB011013\HB001045.D Vial: 12
Acq On : 11-Jan-2013, 03:20 Operator: QM
Sample : E1002-01RE Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jan 11 12:14 2013 Quant Results File: HB011013.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB011013.M
Title :
Last Update : Fri Jan 11 12:05:05 2013
Response via : Multiple Level Calibration
DataAcq Meth : NEWTEST.M

Volume Inj. : 50 ul
Signal Phase : Synergi HYDRO-RP
Signal Info : 250 X 4.60 mm 4 micron

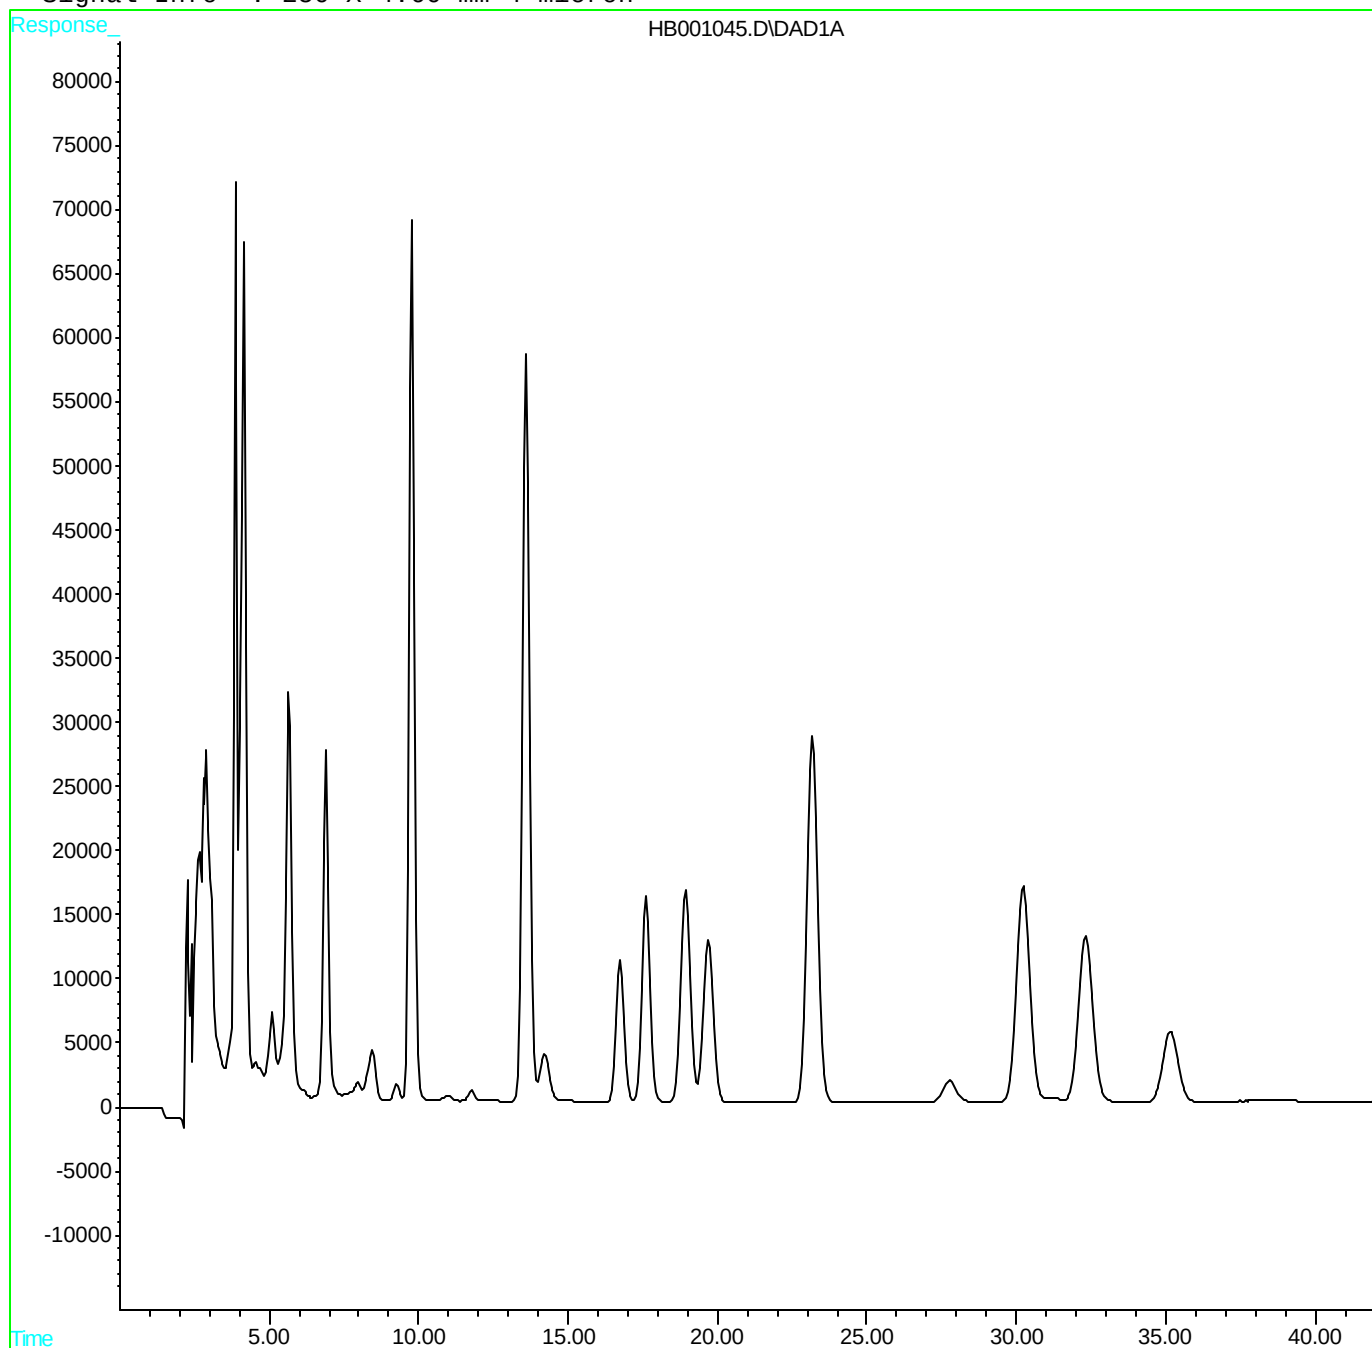

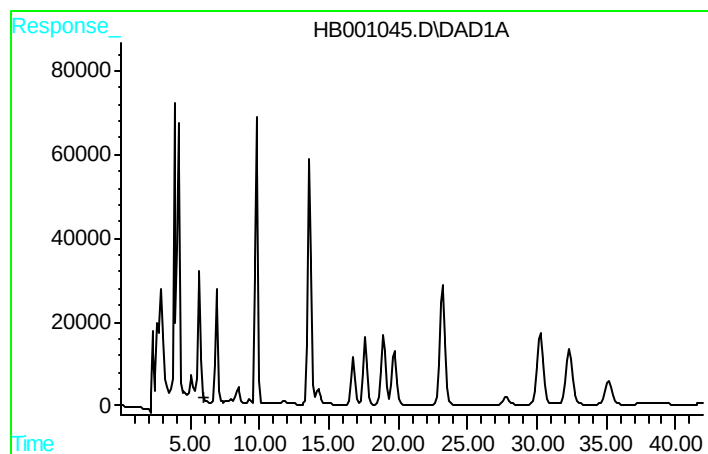

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.