

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001196.D Vial: 6
Acq On : 29-May-2013, 14:24 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:19 2013 Quant Results File: HB052913.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Thu May 30 15:12:10 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	5.00	115869	189.979 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HB001196.D HB052913.M Thu May 30 15:19:01 2013 RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001196.D Vial: 6
Acq On : 29-May-2013, 14:24 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:19 2013 Quant Results File: HB052913.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Thu May 30 15:12:10 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

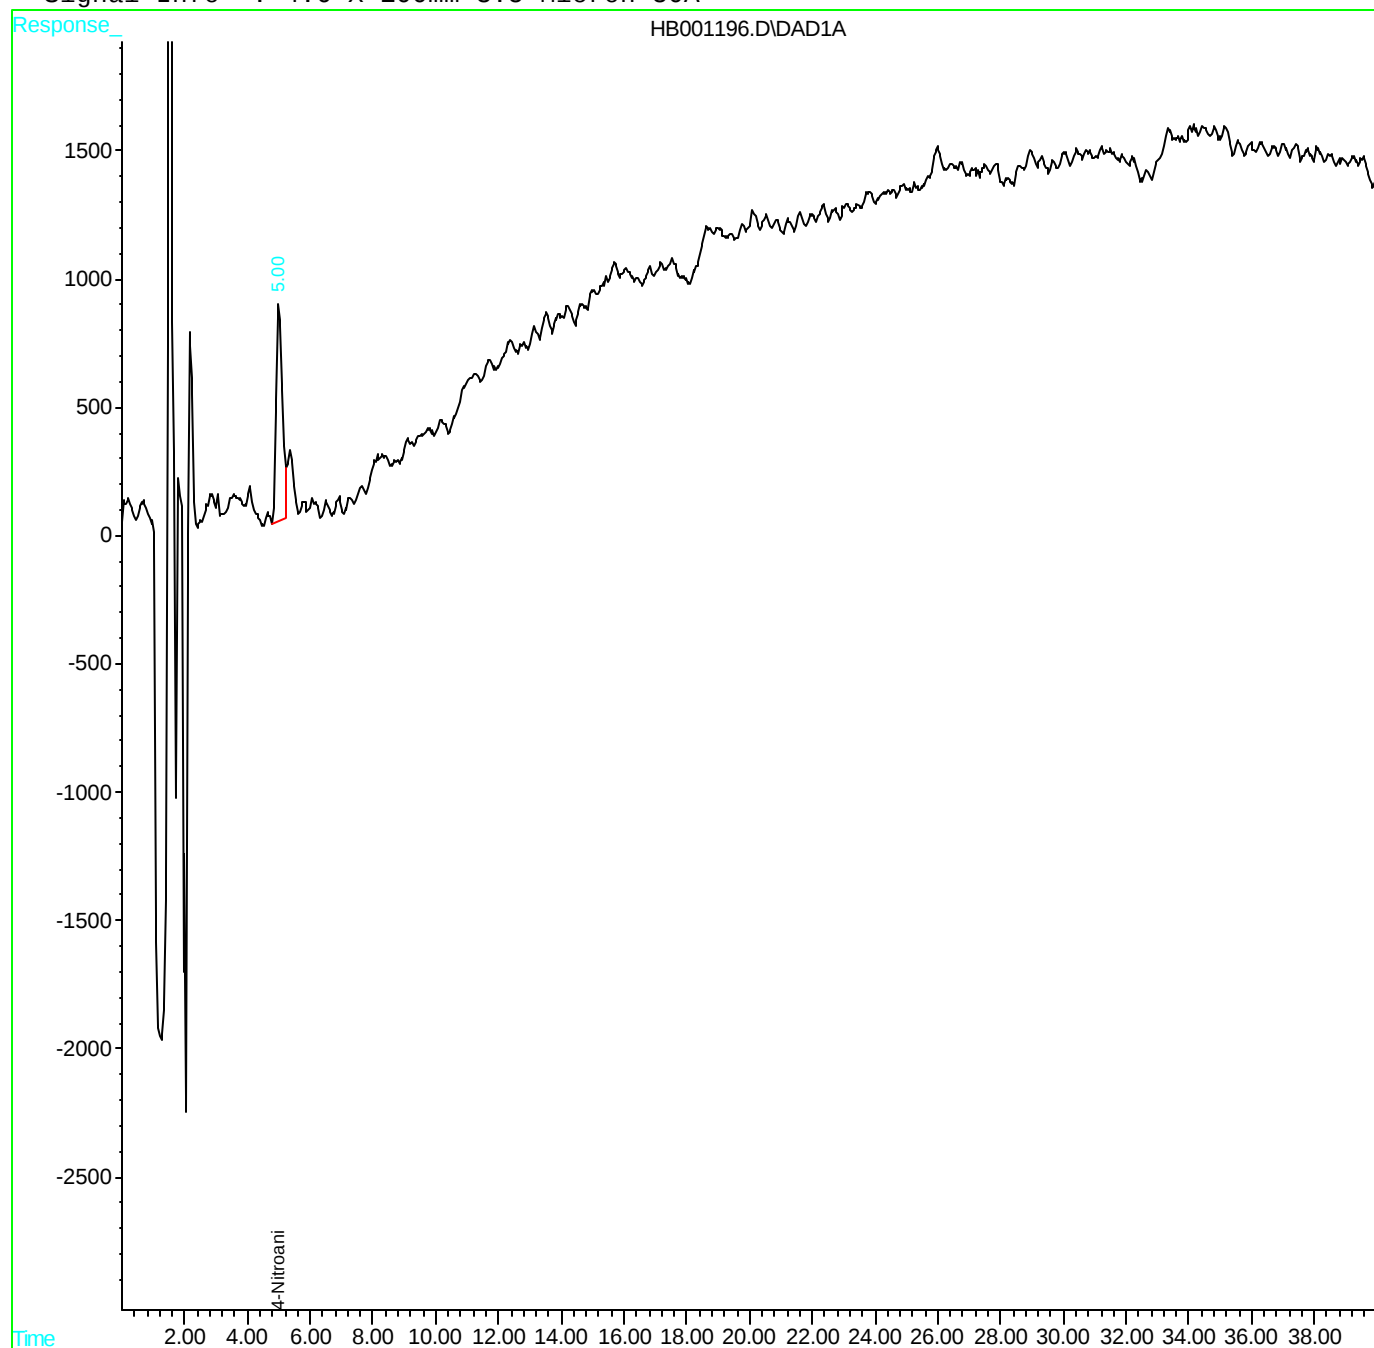

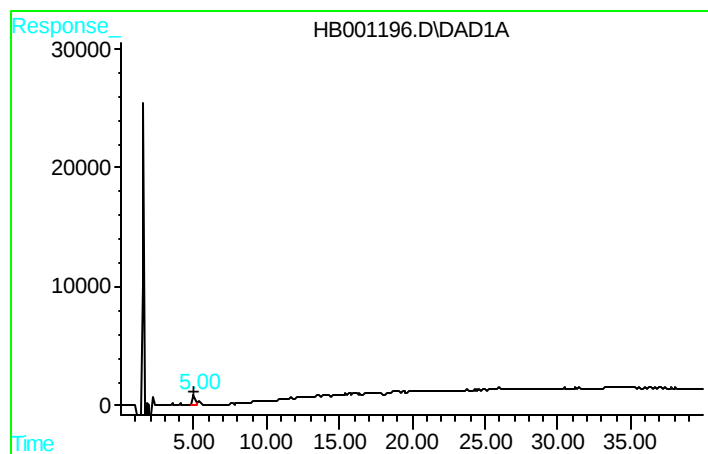

#1 4-Nitroaniline

R.T.: 5.001 min
Delta R.T.: -0.039 min
Response: 115869
Conc: 189.98 ug/L