

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001189.D Vial: 2
Acq On : 29-May-2013, 09:33 Operator: QM
Sample : HMX Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:10 2013 Quant Results File: HB052913.RES

Instrument :
HPLC_B
ClientSampleId :
HMX

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Tue Jan 29 14:25:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.22	50135	82.201 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HB001189.D HB052913.M

Thu May 30 16:31:10 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001189.D Vial: 2
Acq On : 29-May-2013, 09:33 Operator: QM
Sample : HMX Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:10 2013 Quant Results File: HB052913.RES

Instrument :
HPLC_B
ClientSampleId :
HMX

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Tue Jan 29 14:25:38 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

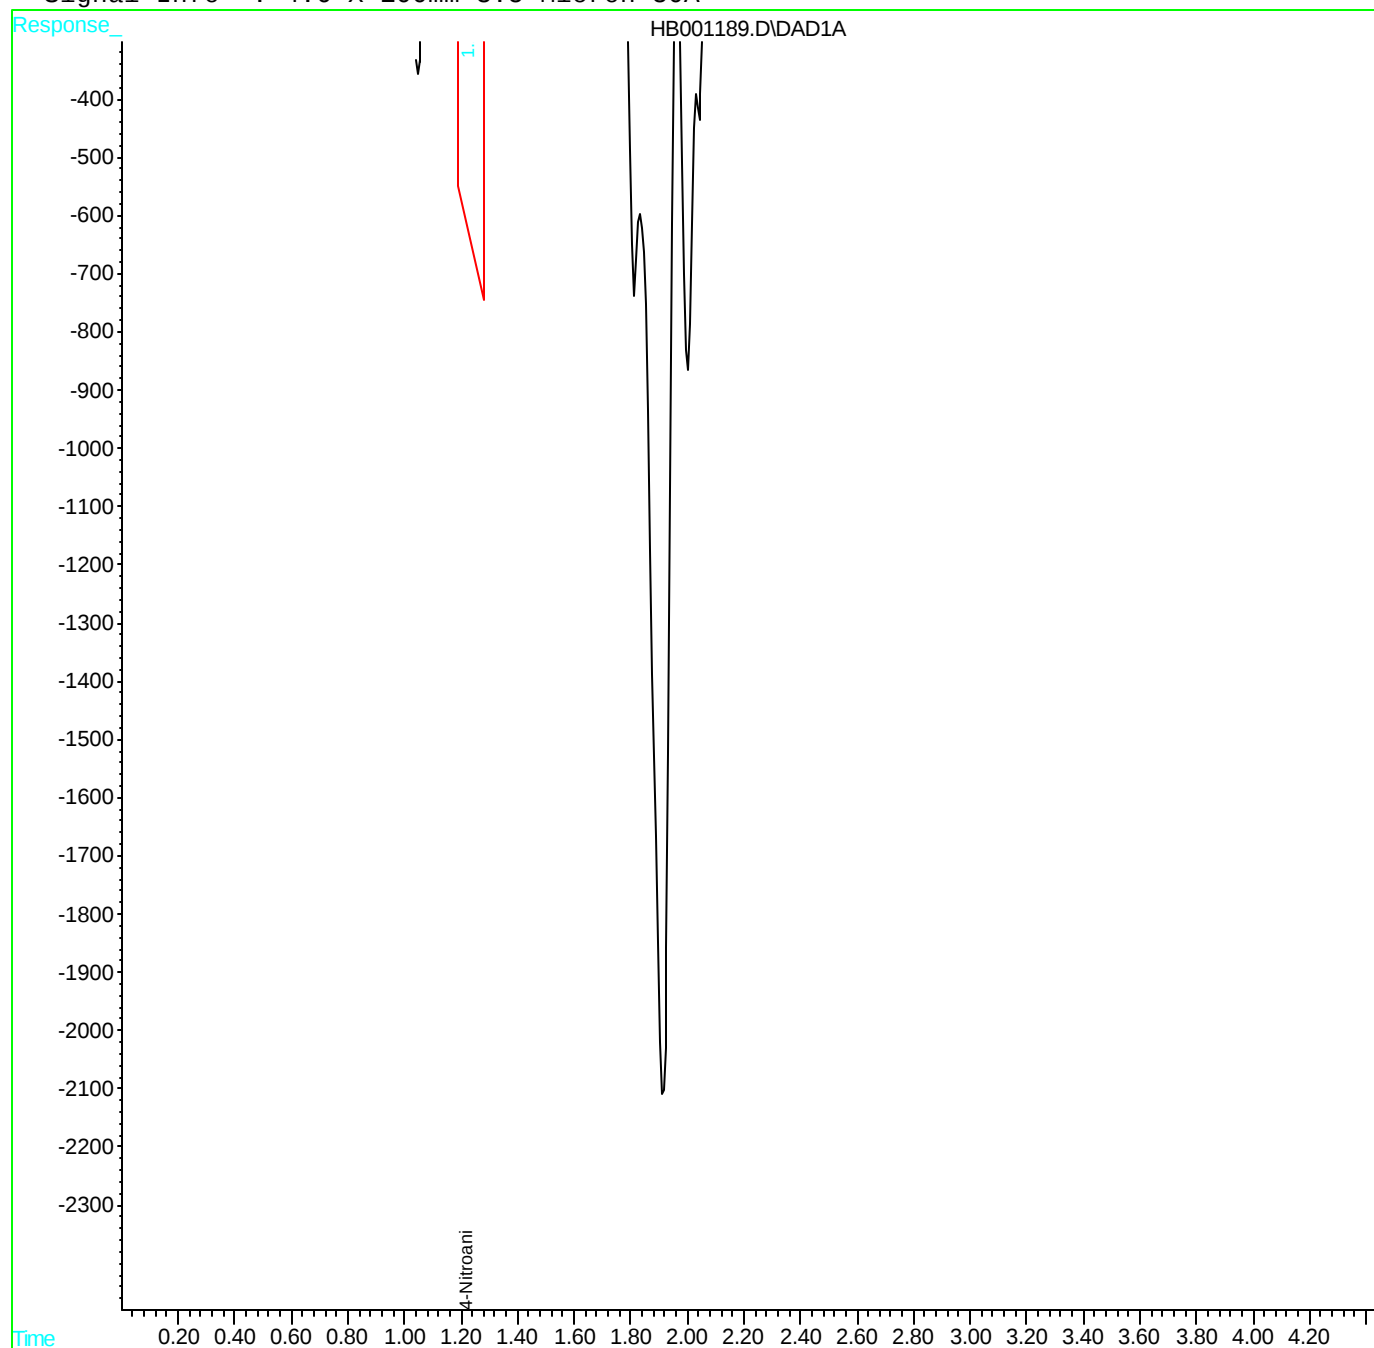

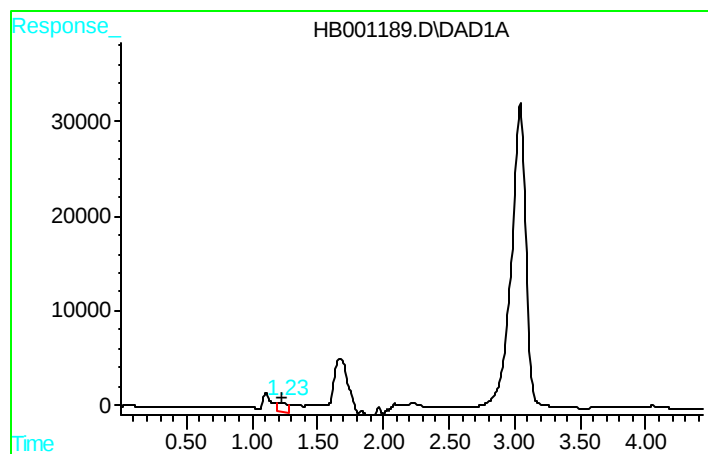

#1 4-Nitroaniline

R.T.: 1.224 min
Delta R.T.: -0.010 min
Response: 50135
Conc: 82.20 ug/L

Instrument :
HPLC_B
ClientSampleId :
HMX