

Data File : Z:\HPCHEM1\HPLC\_B\DATA\HB052913\HB001190.D Vial: 3  
 Acq On : 29-May-2013, 09:39 Operator: QM  
 Sample : SURR. Inst : G1315A  
 Misc : Multiplr: 1.00  
 IntFile : autoint1.e  
 Quant Time: May 30 15:11 2013 Quant Results File: HB052913.RES

Instrument :  
 HPLC\_B  
 ClientSampleId :  
 SURR.

Quant Method : Z:\HPCHEM1\HPLC\_B\METHOD\HB052913.M  
 Title :  
 Last Update : Tue Jan 29 14:25:38 2013  
 Response via : Initial Calibration  
 DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul  
 Signal Phase : ZORBAX Extend-C18  
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
Target Compounds			
3) T RDX	1.54	1304723	1995.372 ug/L

-----  
 Analyst Signature: \_\_\_\_\_ Analyst Name: \_\_\_\_\_ Date: \_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #: \_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #: \_\_\_\_\_

\_\_\_OTHER: \_\_\_\_\_ Compound #: \_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.


Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_B\DATA\HB052913\HB001190.D Vial: 3  
Acq On : 29-May-2013, 09:39 Operator: QM  
Sample : SURR. Inst : G1315A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 30 15:11 2013 Quant Results File: HB052913.RES

Instrument :  
HPLC\_B  
ClientSampled :  
SURR.

Quant Method : Z:\HPCHEM1\HPLC\_B\METHOD\HB052913.M  
Title :  
Last Update : Tue Jan 29 14:25:38 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

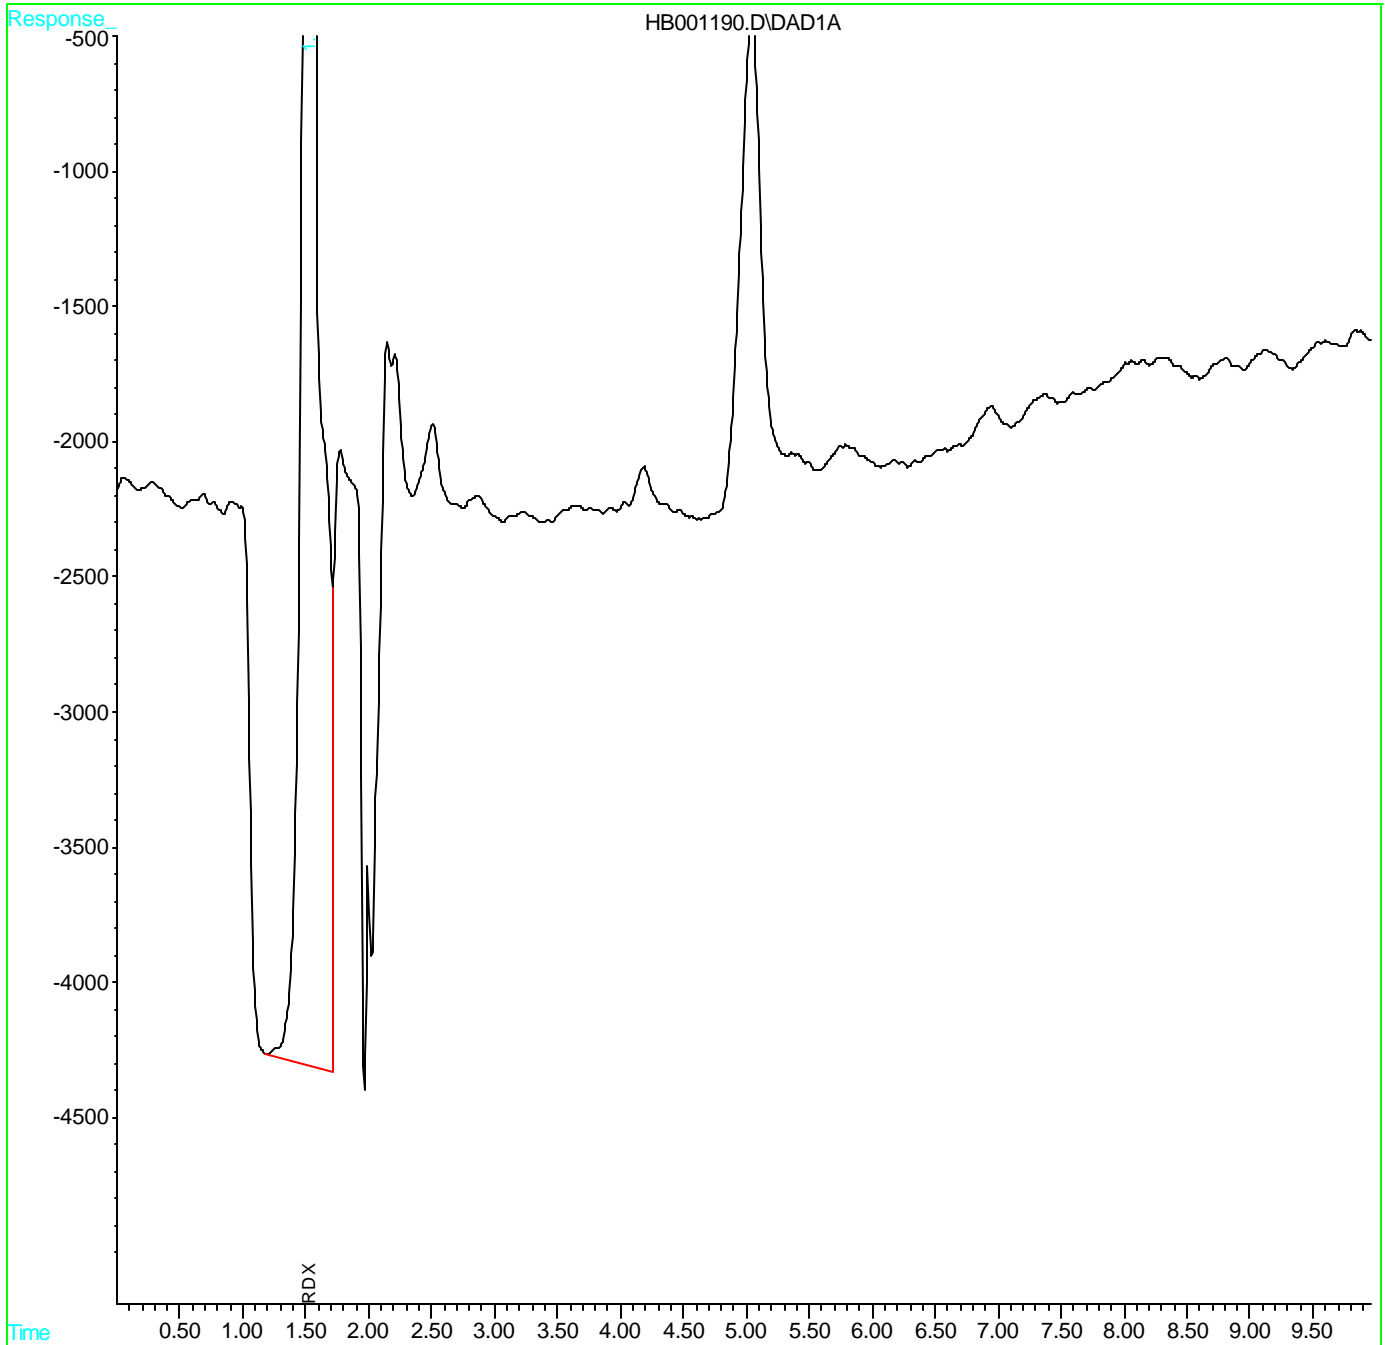


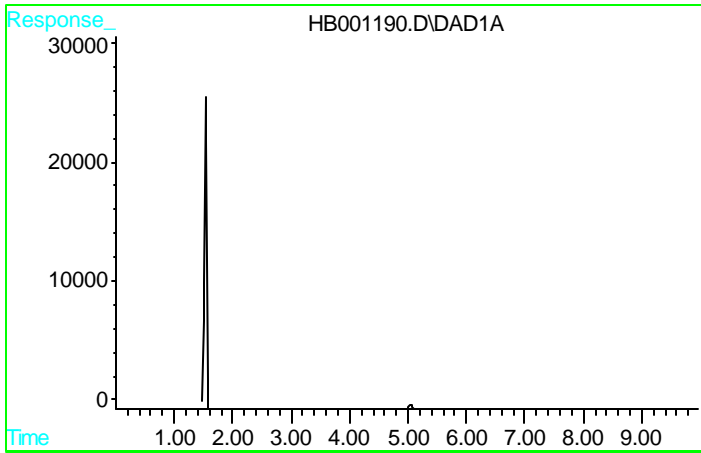

#1 4-Nitroaniline

R.T.: 0.000 min  
 Exp R.T. : 1.234 min  
 Response: 0  
 Conc: N.D.

Instrument :  
 HLPC\_B  
 ClientSampled :  
 SURR.

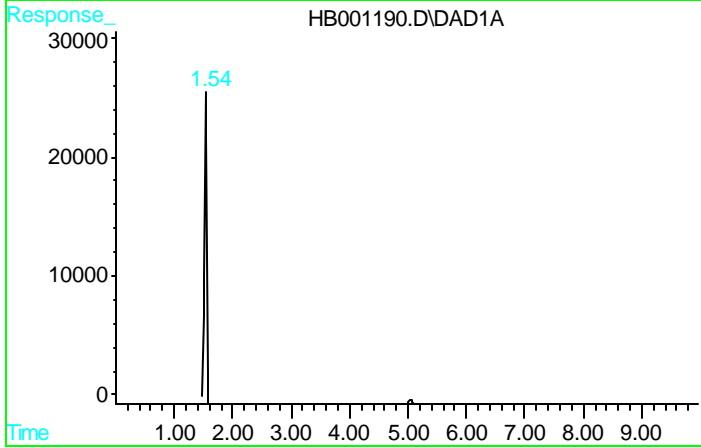

#3 RDX

R.T.: 1.539 min  
 Delta R.T.: -0.056 min  
 Response: 1304723  
 Conc: 1995.37 ug/L