

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001196.D Vial: 6
Acq On : 29-May-2013, 14:24 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:35 2013 Quant Results File: HB052913.RES

Instrument :
HPLC_B
LabSampleId :
HSTDICC0020

Manual Integrations
APPROVED

mohammad
5/31/2013 5:30:15 PM

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Thu May 30 15:12:10 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2) T	HMX	3.05	5350	6.327 ug/L m
3) T	RDX	6.06	5171	7.909 ug/L m

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HB001196.D HB052913.M Thu May 30 16:43:53 2013 RPT1

Quantitation Report

Data File : Z:\HPCHEM1\HPLC_B\DATA\HB052913\HB001196.D Vial: 6
Acq On : 29-May-2013, 14:24 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 30 15:35 2013 Quant Results File: HB052913.RES


Instrument :
HPLC_B
LabSampleId :
HSTDICC0020


Manual Integrations
APPROVED

mohammad
5/31/2013 5:30:15 PM

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB052913.M
Title :
Last Update : Thu May 30 15:12:10 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

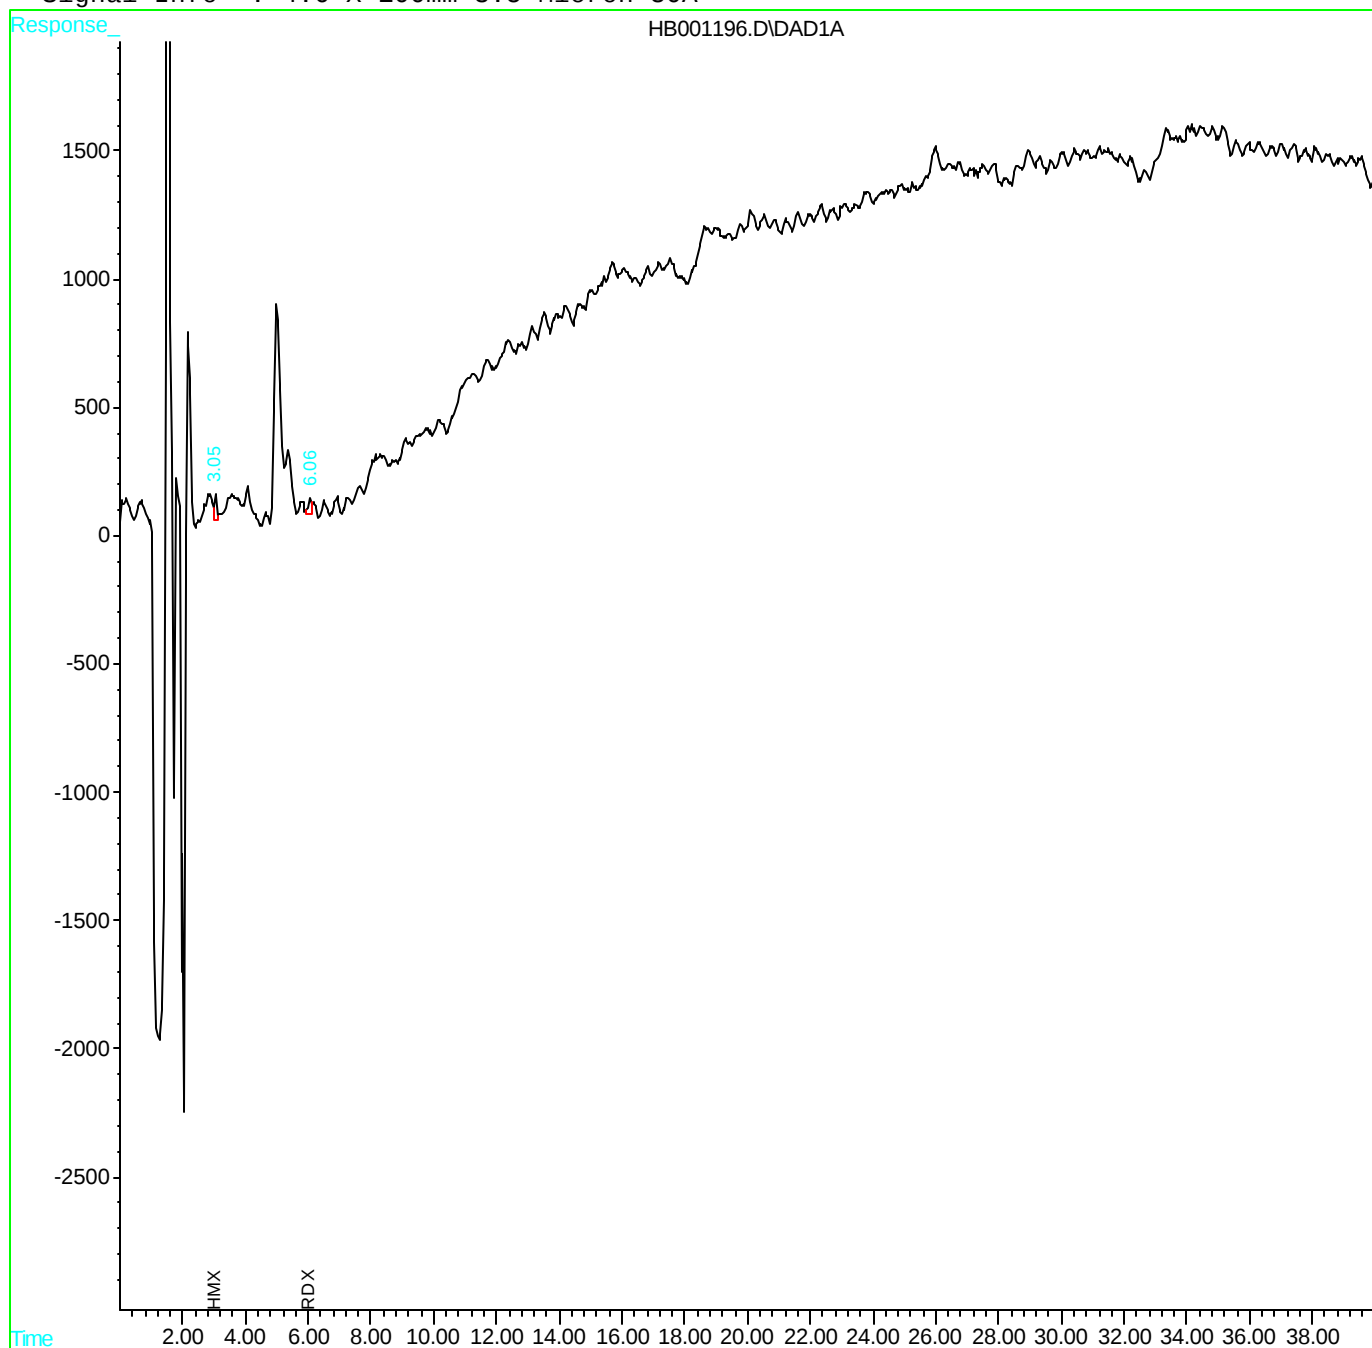

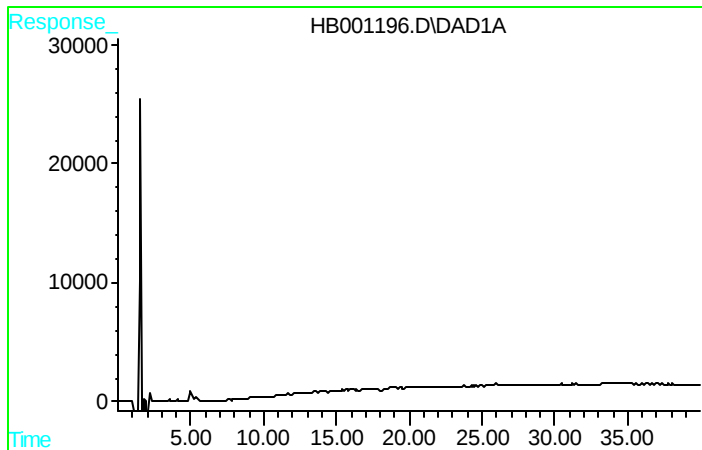


#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 5.040 min
Response: 0
Conc: N.D.

Instrument :
HPLC_B
LabSampleId :
HSTDIC0020


Manual Integrations
APPROVED

mohammad
5/31/2013 5:30:15 PM

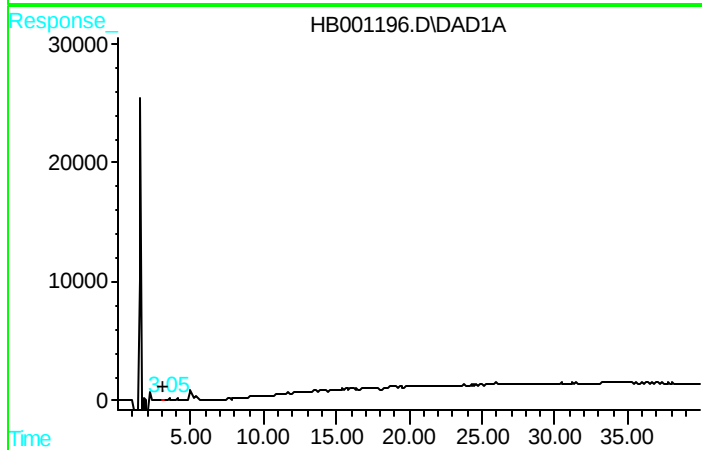

#2 HMX

R.T.: 3.048 min
Delta R.T.: 0.007 min
Response: 5350
Conc: 6.33 ug/L m

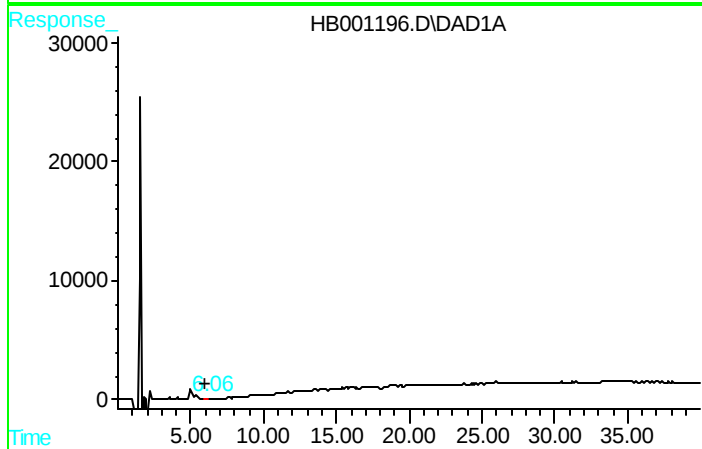

#3 RDX

R.T.: 6.057 min
Delta R.T.: 0.027 min
Response: 5171
Conc: 7.91 ug/L m