

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001346.D Vial: 6
Acq On : 15-Jul-2013, 14:29 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 15 18:05 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 17:52:31 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3) T	2,4-Dinitrotoluene	24.49	25710	35.095 ug/L
------	--------------------	-------	-------	-------------

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HB001346.D HB071513.M Mon Jul 15 18:05:43 2013 RPT1


Quantitation Report

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001346.D Vial: 6
Acq On : 15-Jul-2013, 14:29 Operator: QM
Sample : HSTDICC0020 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 15 18:05 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 17:52:31 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M


Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

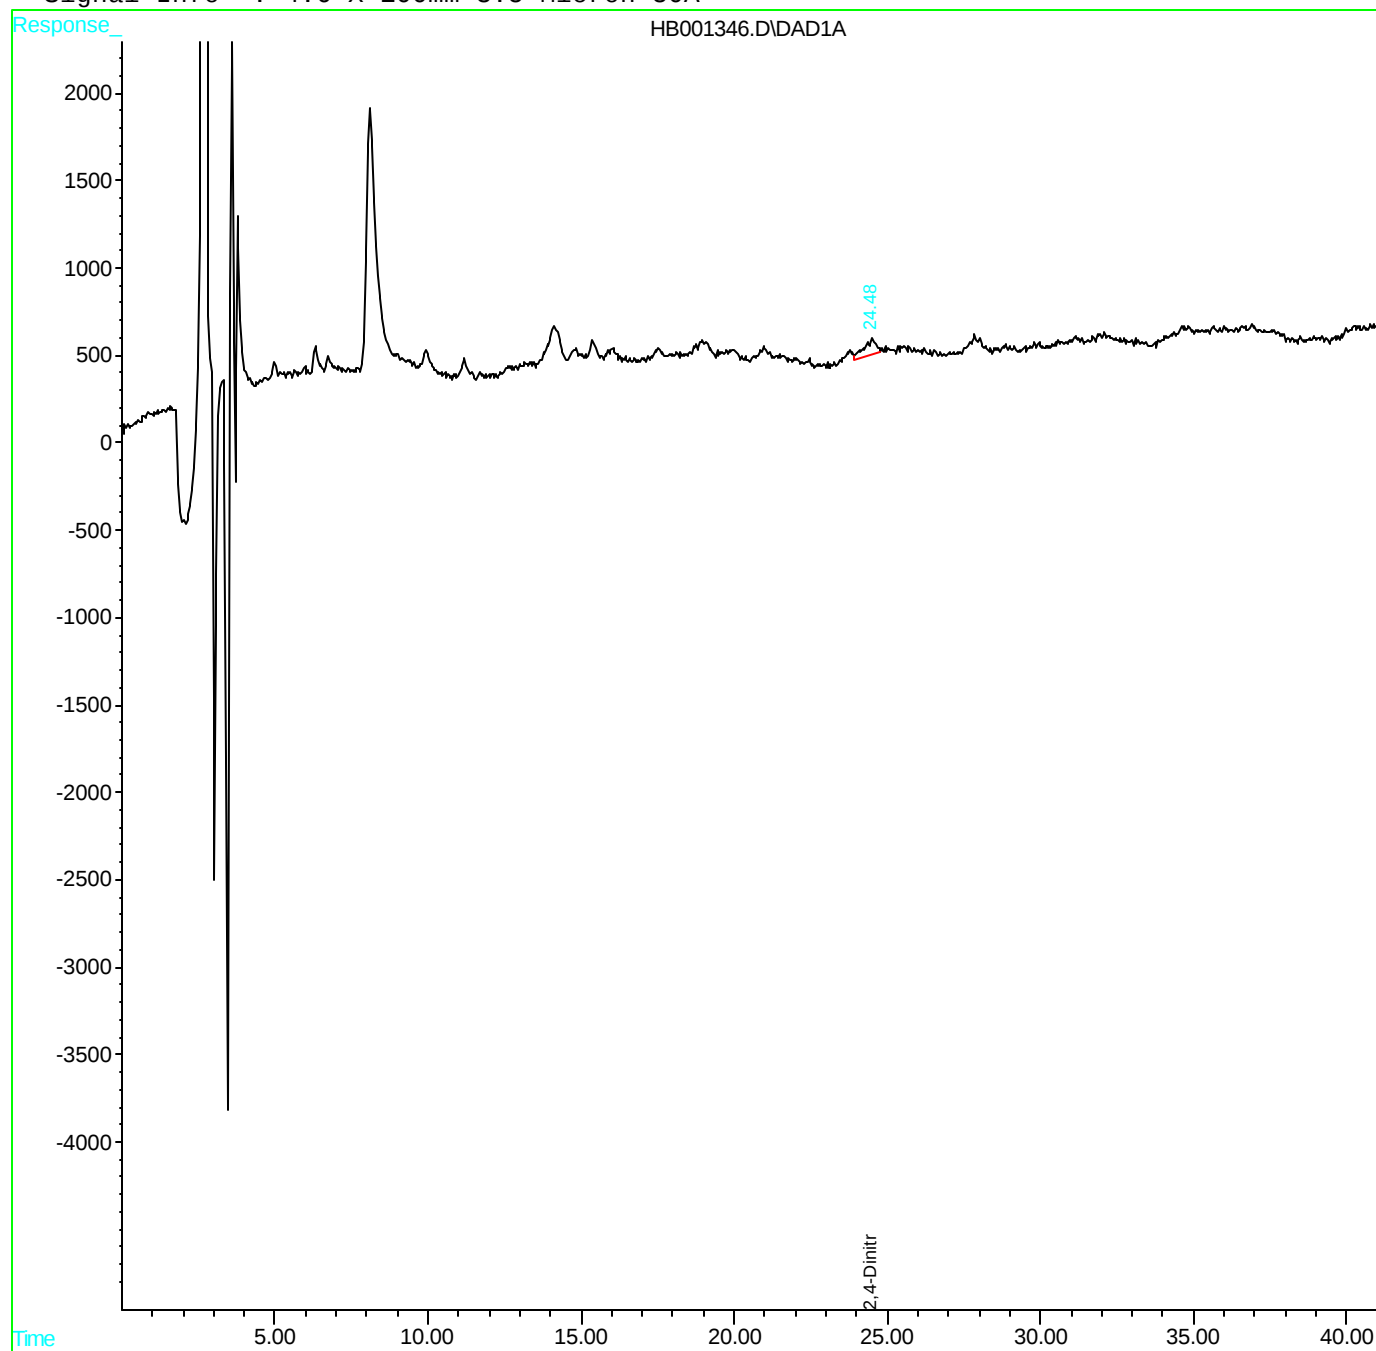

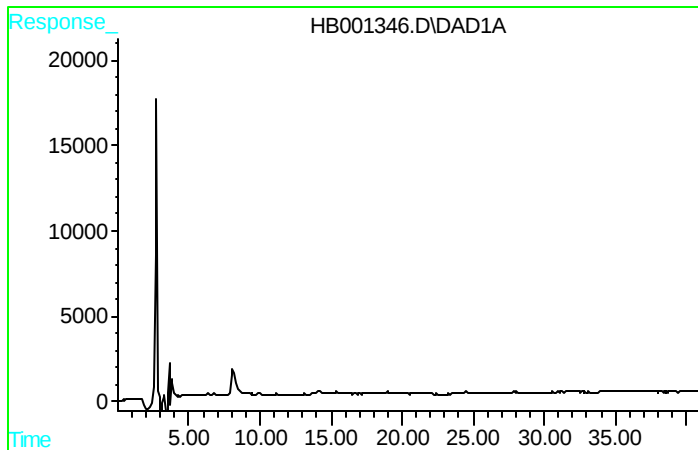

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 6.770 min
Response: 0
Conc: N.D.

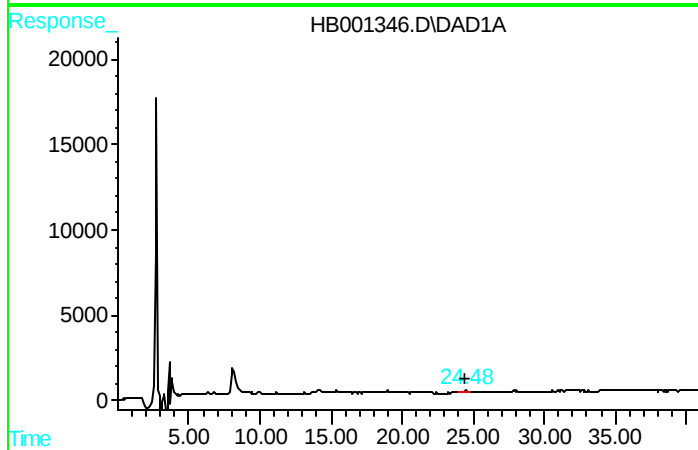

#3 2,4-Dinitrotoluene

R.T.: 24.492 min
Delta R.T.: 0.022 min
Response: 25710
Conc: 35.09 ug/L