

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001352.D Vial: 1
Acq On : 15-Jul-2013, 18:43 Operator: QM
Sample : HSTDCCC0500 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 16 10:31 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 18:08:55 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	6.74	271010	576.621 ug/L
Target Compounds			
2) T HMX	4.97	240326	544.021 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HB001352.D HB071513.M Tue Jul 16 10:31:26 2013 RPT1


Quantitation Report

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001352.D Vial: 1
Acq On : 15-Jul-2013, 18:43 Operator: QM
Sample : HSTDCCC0500 Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 16 10:31 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 18:08:55 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M


Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

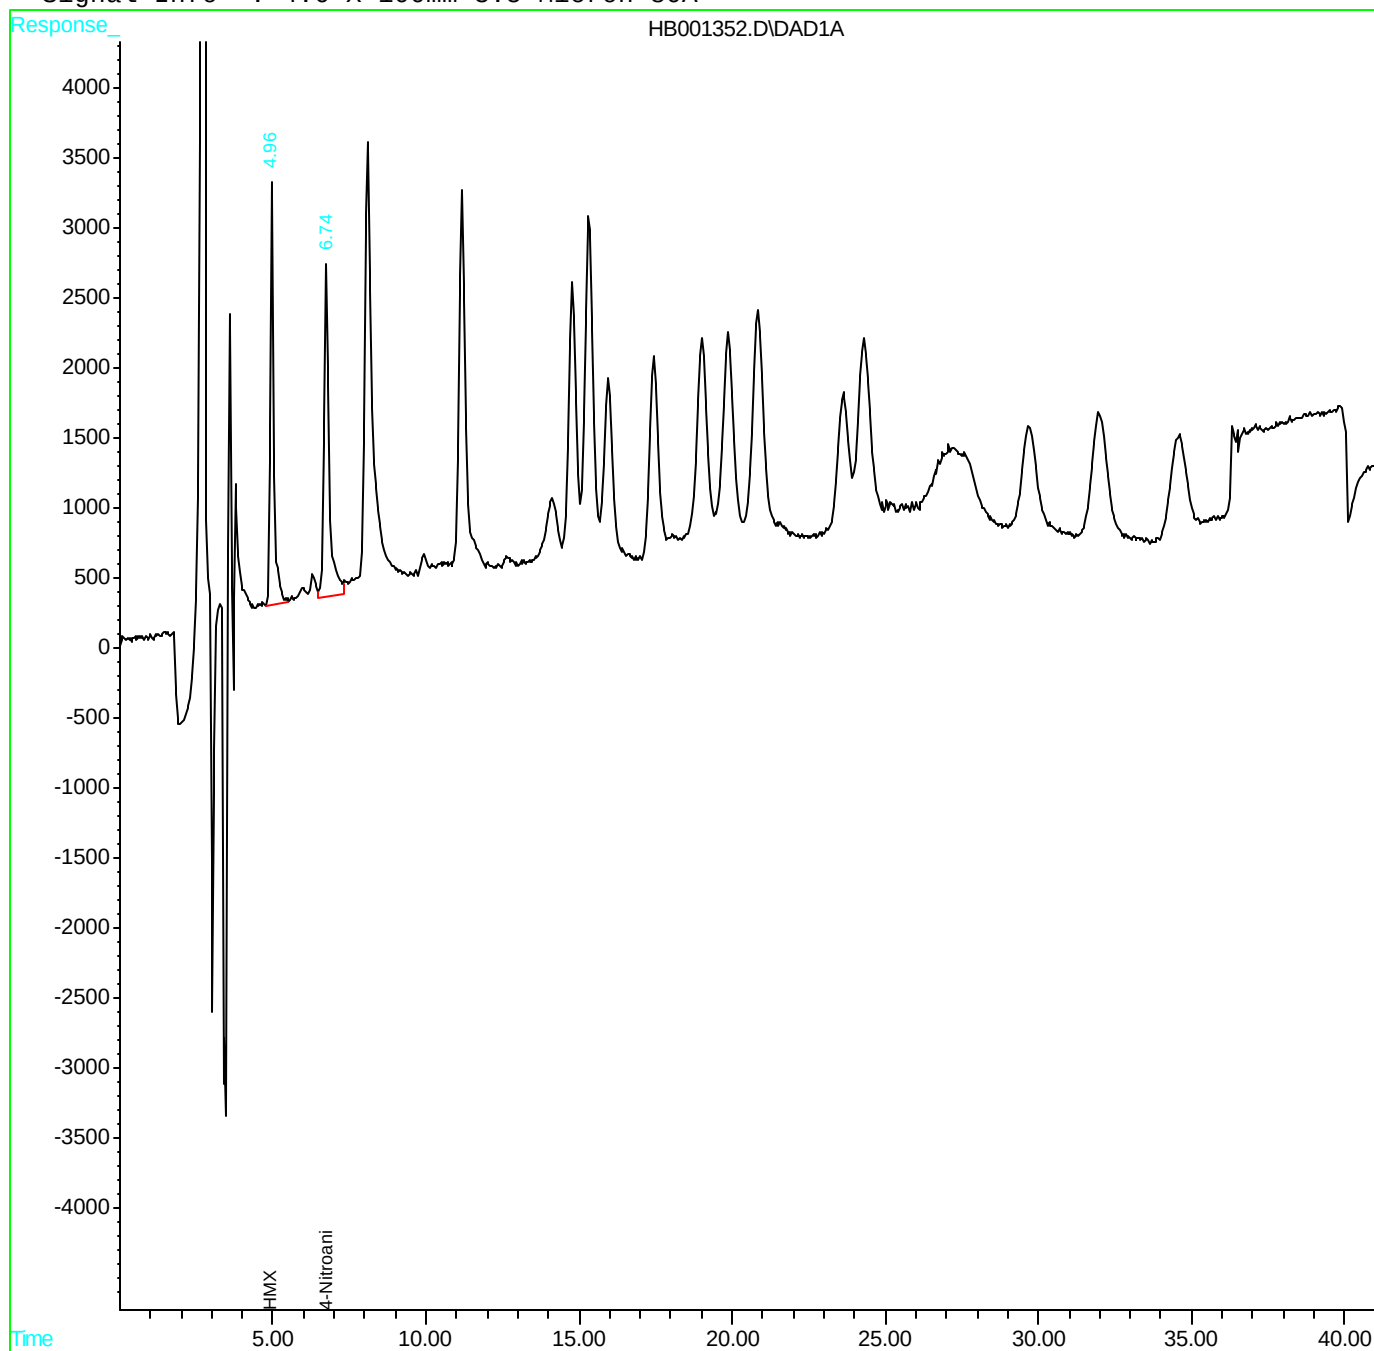

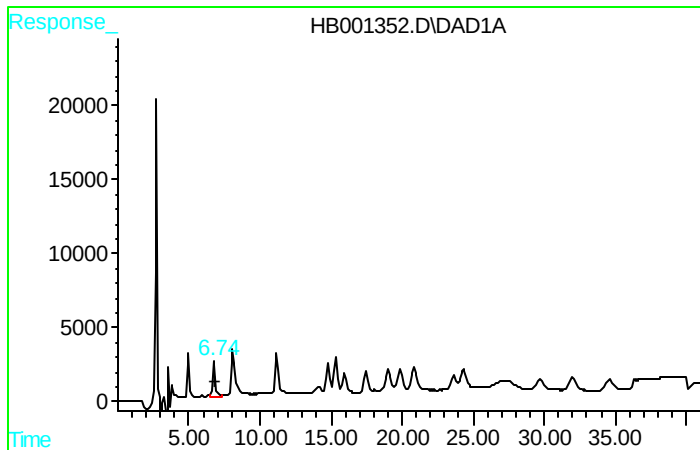

#1 4-Nitroaniline

R.T.: 6.742 min
Delta R.T.: -0.028 min
Response: 271010
Conc: 576.62 ug/L

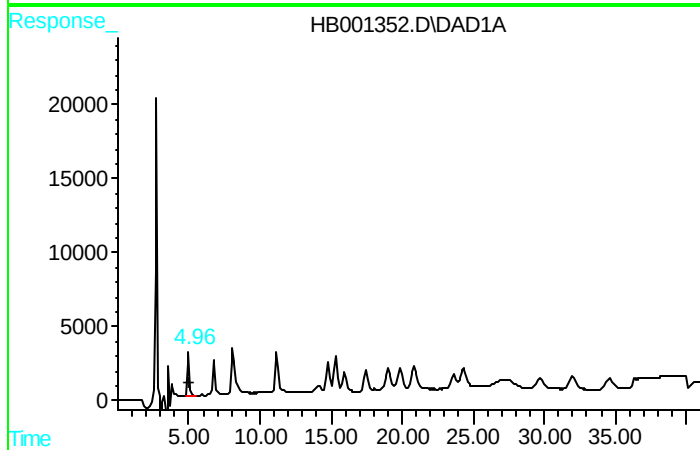

#2 HMX

R.T.: 4.966 min
Delta R.T.: -0.014 min
Response: 240326
Conc: 544.02 ug/L