

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001353.D Vial: 11
Acq On : 15-Jul-2013, 19:26 Operator: QM
Sample : 2,4-DNT Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 16 10:32 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 18:08:55 2013
Response via : Initial Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HB001353.D HB071513.M Tue Jul 16 10:53:47 2013 RPT1


Quantitation Report

Data File : S:\HPCHEM1\HPLC_B\DATA\HB071513\HB001353.D Vial: 11
Acq On : 15-Jul-2013, 19:26 Operator: QM
Sample : 2,4-DNT Inst : G1315A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 16 10:32 2013 Quant Results File: HB071513.RES

Quant Method : Z:\HPCHEM1\HPLC_B\METHOD\HB071513.M
Title :
Last Update : Mon Jul 15 18:08:55 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BCON.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

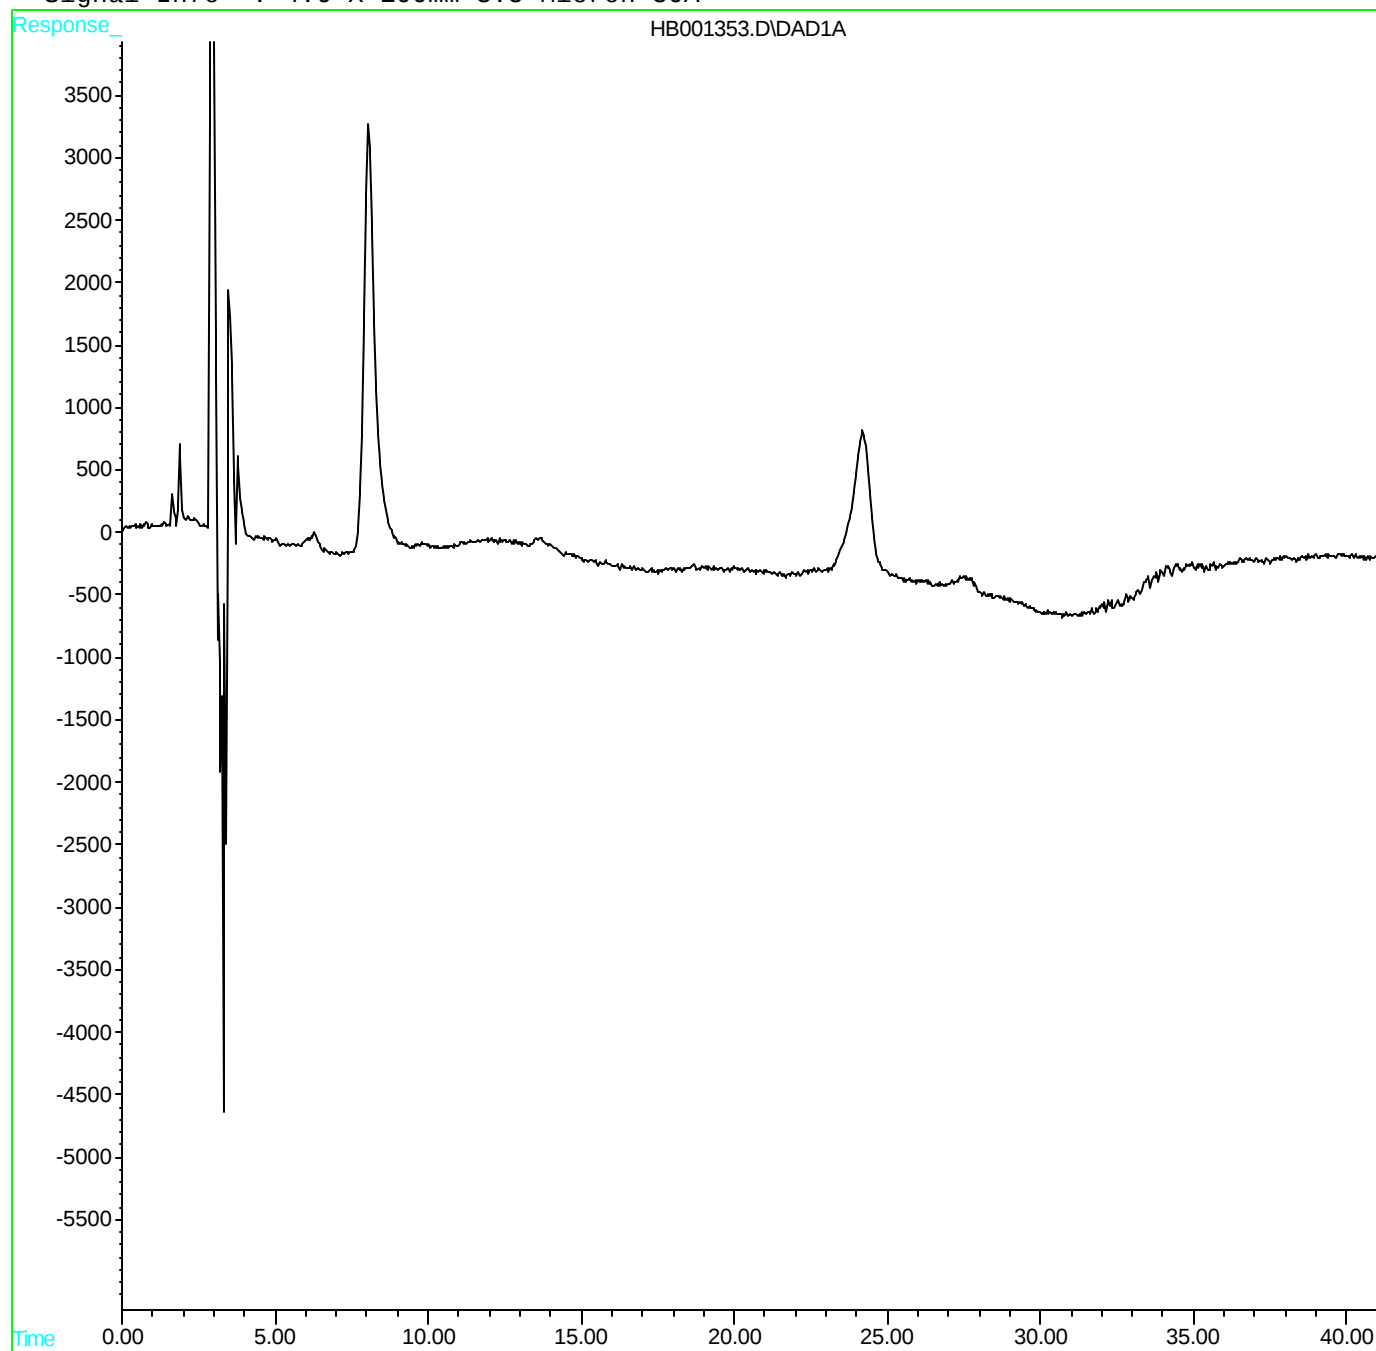

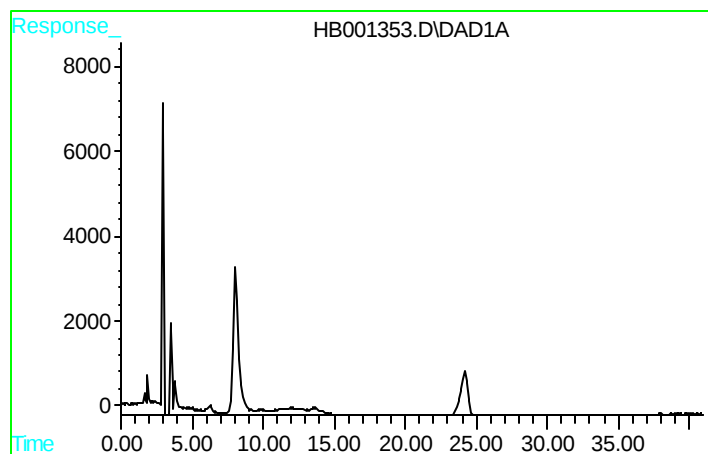

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 6.770 min
Response: 0
Conc: N.D.