

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004003.D Vial: 23
Acq On : 03-Jan-2013, 23:52 Operator: HLM
Sample : PB67749BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 4 13:30 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
PB67749BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.37	667624	185.632 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 61.88%

Target Compounds

17) T	Nitroglycerin	6.21	165542	2887.332 ug/L
-------	---------------	------	--------	---------------

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004003.D

Vial: 23

Acq On : 03-Jan-2013, 23:52

Operator: HLM

Sample : PB67749BS2

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 4 13:30 2013 Quant Results File: HL010313.RES

Instrument :

HPLC_L

ClientSampleId :

PB67749BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Fri Jan 04 13:29:03 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

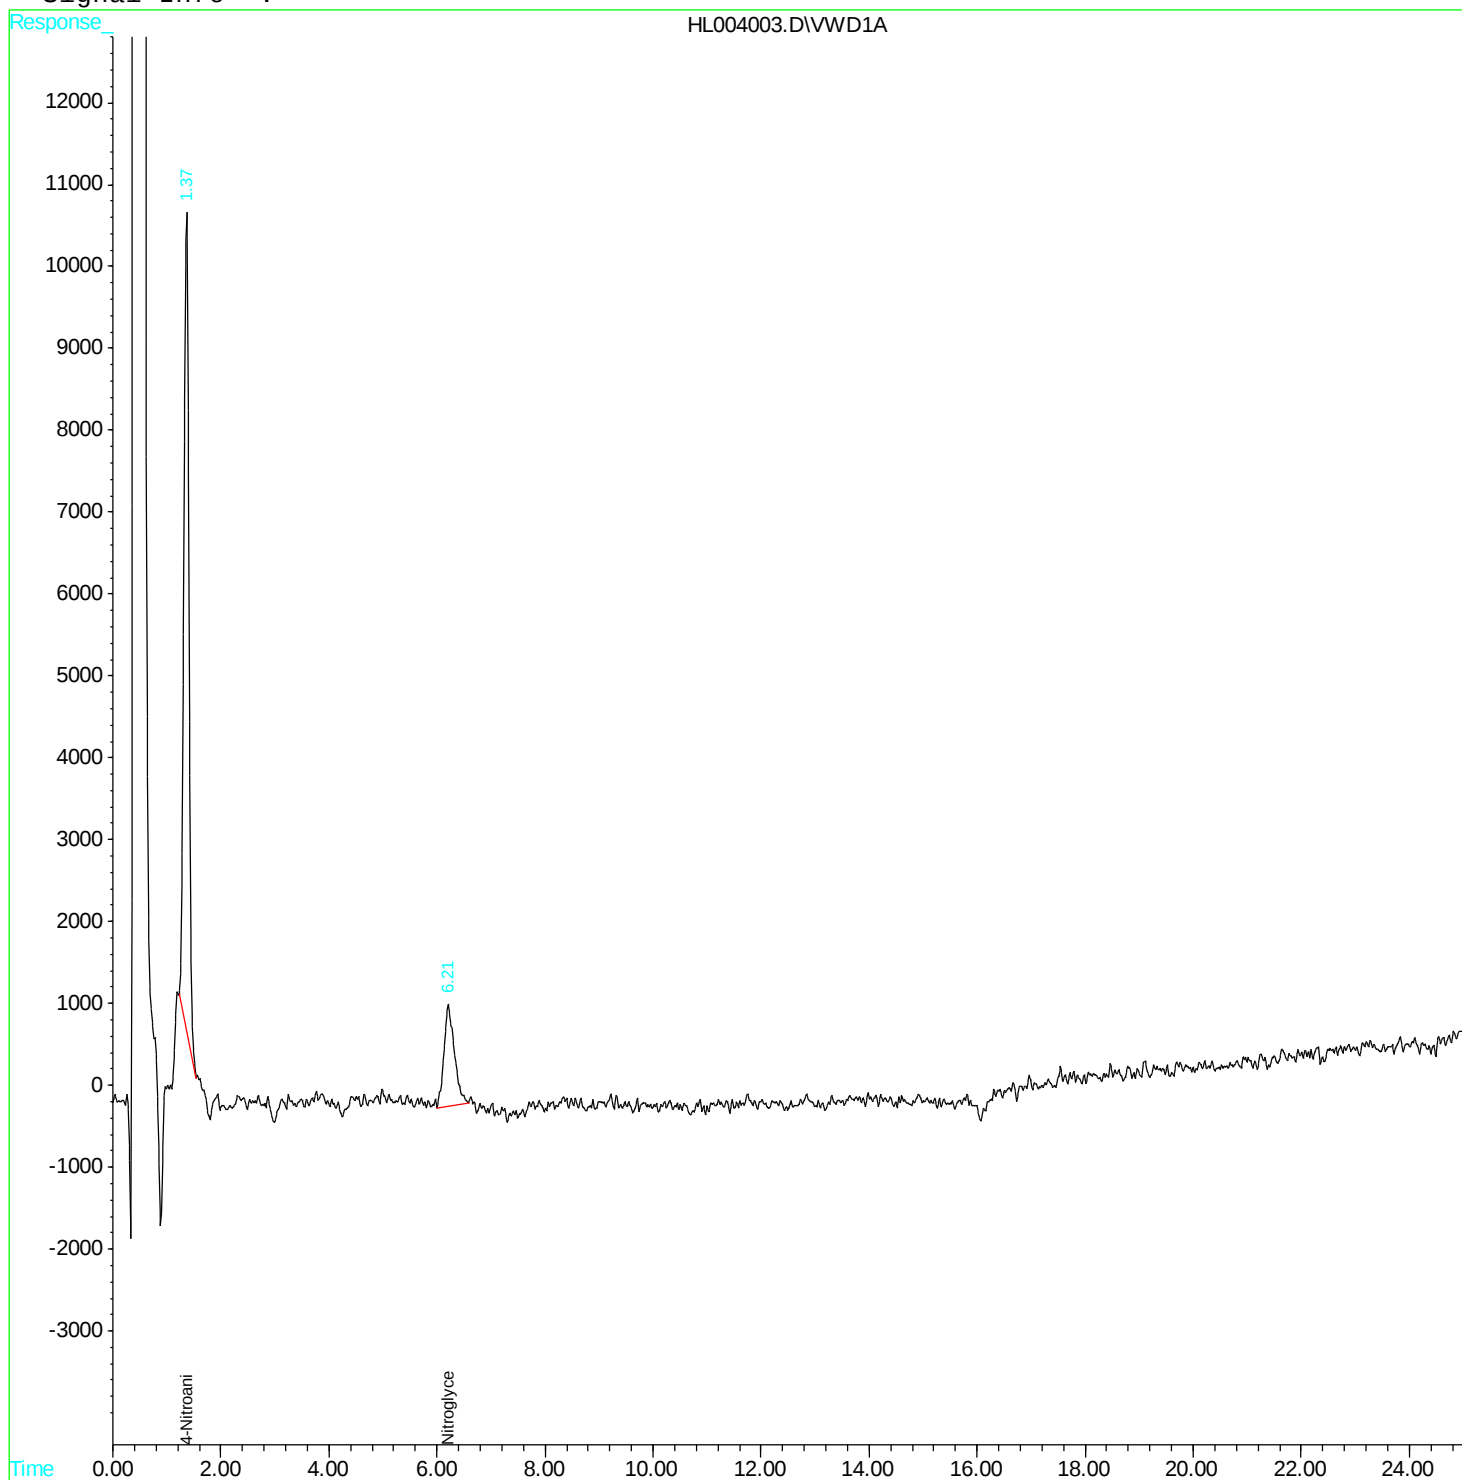

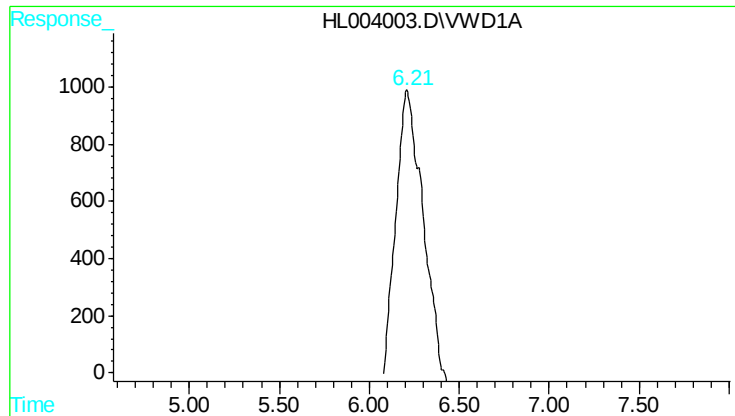

#17 Nitroglycerin

R.T.: 6.210 min
Delta R.T.: -0.016 min
Response: 165542
Conc: 2887.33 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67749BS2