

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004006.D Vial: 26
Acq On : 04-Jan-2013, 01:13 Operator: HLM
Sample : D5191-01MS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 4 13:30 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
MRSNORTH1-01-ISM-3MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.37	1091823	303.580 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 101.19%

Target Compounds

17) T	Nitroglycerin	6.24	162521	2834.633 ug/L
-------	---------------	------	--------	---------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\130103\HL004006.D Vial: 26
 Acq On : 04-Jan-2013, 01:13 Operator: HLM
 Sample : D5191-01MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 4 13:30 2013 Quant Results File: HL010313.RES

Instrument :
 HPLC_L
 ClientSampleId :
 MRSNORTH1-01-ISM-3MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Fri Jan 04 13:29:03 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

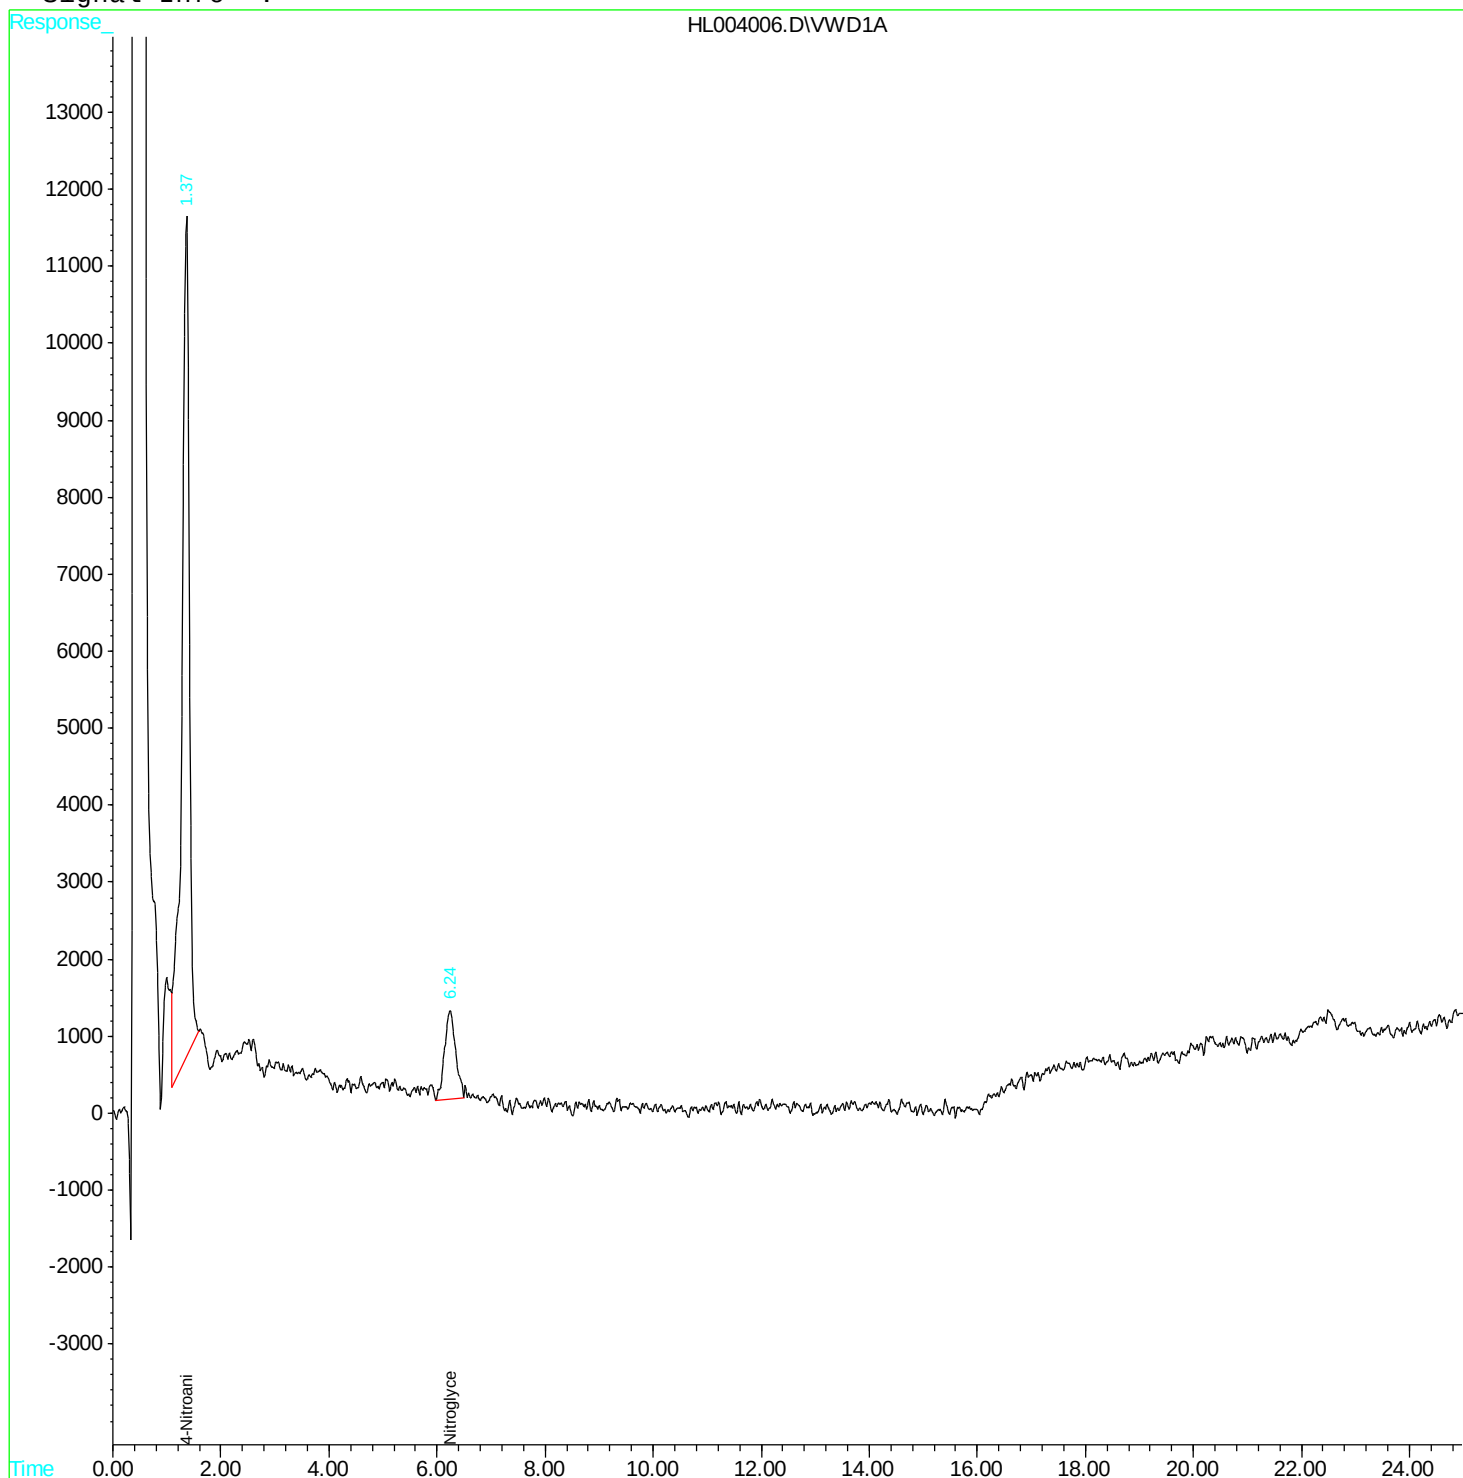

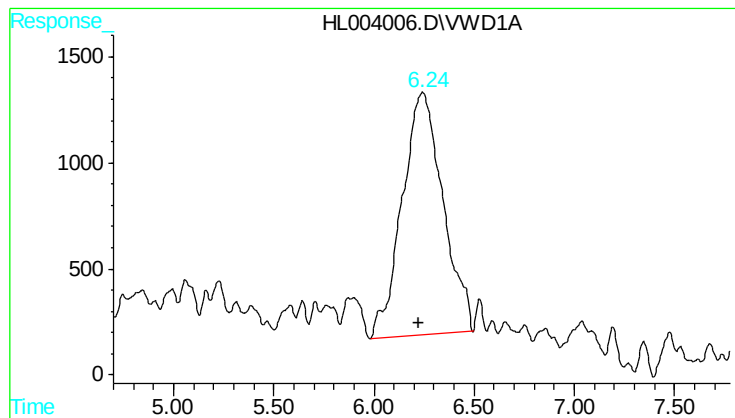

#17 Nitroglycerin

R.T.: 6.244 min
Delta R.T.: 0.018 min
Response: 162521
Conc: 2834.63 ug/L

Instrument :
HPLC_L
ClientSampleId :
MRSNORTH1-01-ISM-3MS2