

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004008.D Vial: 28  
Acq On : 04-Jan-2013, 02:07 Operator: HLM  
Sample : D5191-01MSD2 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Jan 4 13:31 2013 Quant Results File: HL010313.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
MRSNORTH1-01-ISM-3MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Fri Jan 04 13:29:03 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

|               |                |       |          |                   |
|---------------|----------------|-------|----------|-------------------|
| 1) S          | 4-Nitroaniline | 1.37  | 641548   | 178.381 ug/L      |
| Spiked Amount | 300.000        | Range | 37 - 149 | Recovery = 59.46% |

Target Compounds

|       |               |      |        |               |
|-------|---------------|------|--------|---------------|
| 17) T | Nitroglycerin | 6.21 | 121623 | 2121.308 ug/L |
|-------|---------------|------|--------|---------------|


# Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\130103\HL004008.D Vial: 28  
 Acq On : 04-Jan-2013, 02:07 Operator: HLM  
 Sample : D5191-01MSD2 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Jan 4 13:31 2013 Quant Results File: HL010313.RES

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 MRSNORTH1-01-ISM-3MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)  
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
 Last Update : Fri Jan 04 13:29:03 2013  
 Response via : Multiple Level Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. :  
 Signal Phase :  
 Signal Info :

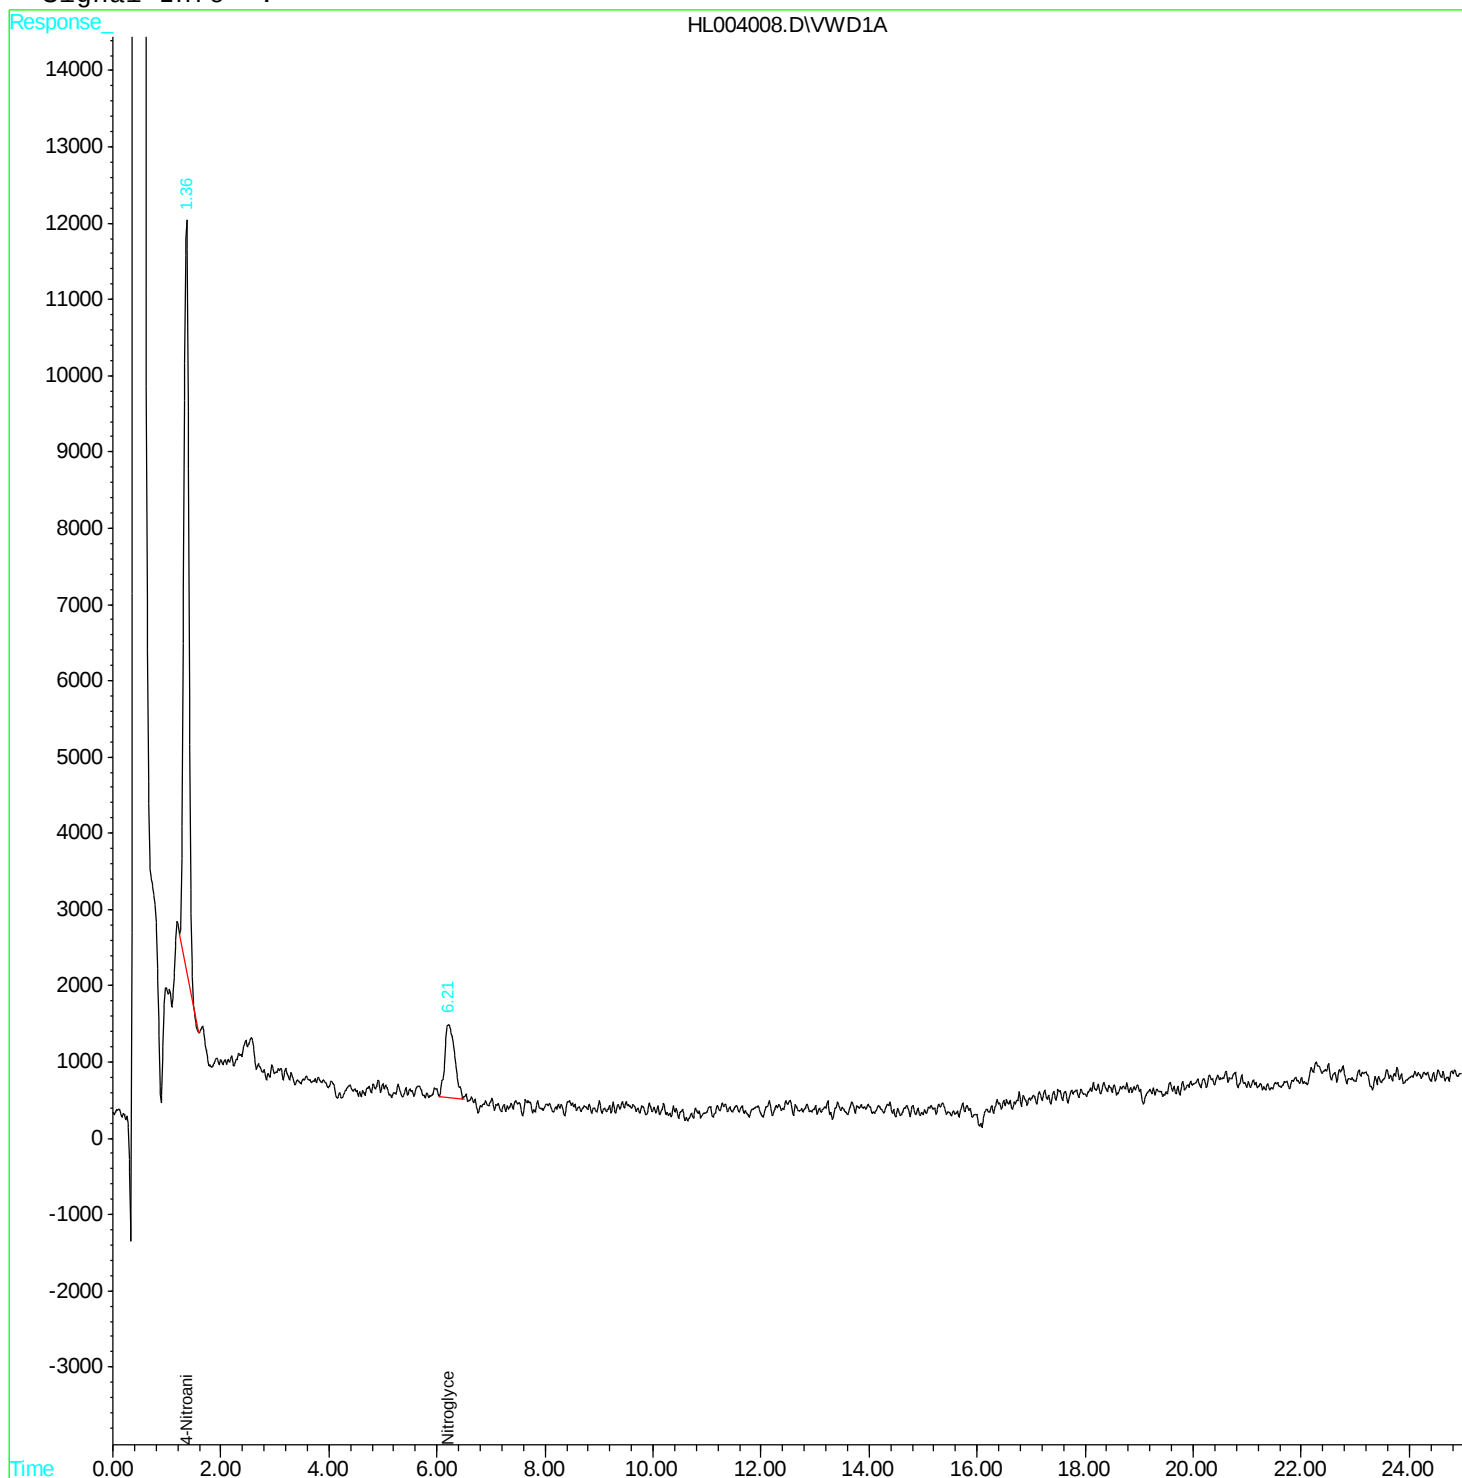

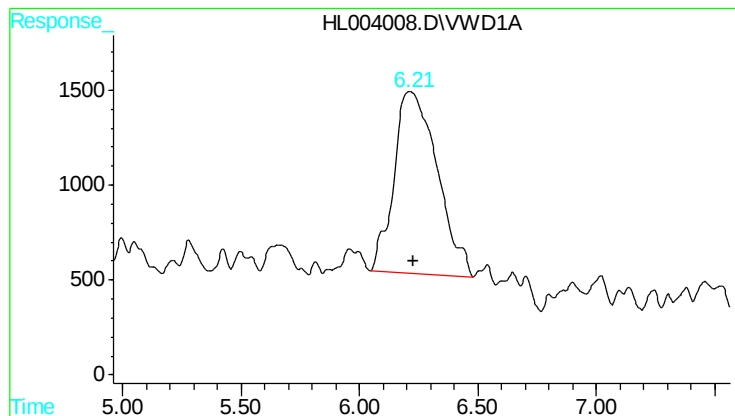

#17 Nitroglycerin

R.T.: 6.213 min  
Delta R.T.: -0.013 min  
Response: 121623  
Conc: 2121.31 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
MRSNORTH1-01-ISM-3MSD2