

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004012.D Vial: 5
 Acq On : 04-Jan-2013, 03:54 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 4 13:31 2013 Quant Results File: HL010313.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Fri Jan 04 13:29:03 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.37	3667770	1019.818 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 339.94%#

Target Compounds

2) T	HMX	0.92	4047649	941.889 ug/L
3) T	RDX	1.77	5528575	1040.936 ug/L
4) T	1,3,5-Trinitrobenzene	2.76	5809934	492.788 ug/L
5) T	Tetryl	6.32	8193622	989.226 ug/L
6) T	2,4,6-Trinitrotoluene	6.68	5627856	504.760 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.17	5324129	505.302 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.50	3696316	508.026 ug/L
9) T	2,4-Dinitrotoluene	8.34	7547602	491.169 ug/L
10) T	2,6-Dinitrotoluene	8.73	4289993	506.856 ug/L
11) T	1,3-Dinitrobenzene	3.67	8158968	494.201 ug/L
12) T	Nitrobenzene	4.93	5251271	484.713 ug/L
13) T	2-Nitrotoluene	12.03	6437122	968.192 ug/L
14) T	3-Nitrotoluene	14.10	6899086	976.481 ug/L
15) T	4-Nitrotoluene	12.81	5459798	976.607 ug/L
16) T	3,5-Dinitroaniline	4.02	15734396	980.477 ug/L
18) T	PETN	19.29	22419919	2476.404 ug/L

Data File : H:\VOL1\HPLC\HPLC L\130103\HL004012.D

Vial: 5

Acq On : 04-Jan-2013, 03:54

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 4 13:31 2013 Quant Results File: HL010313.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Fri Jan 04 13:29:03 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

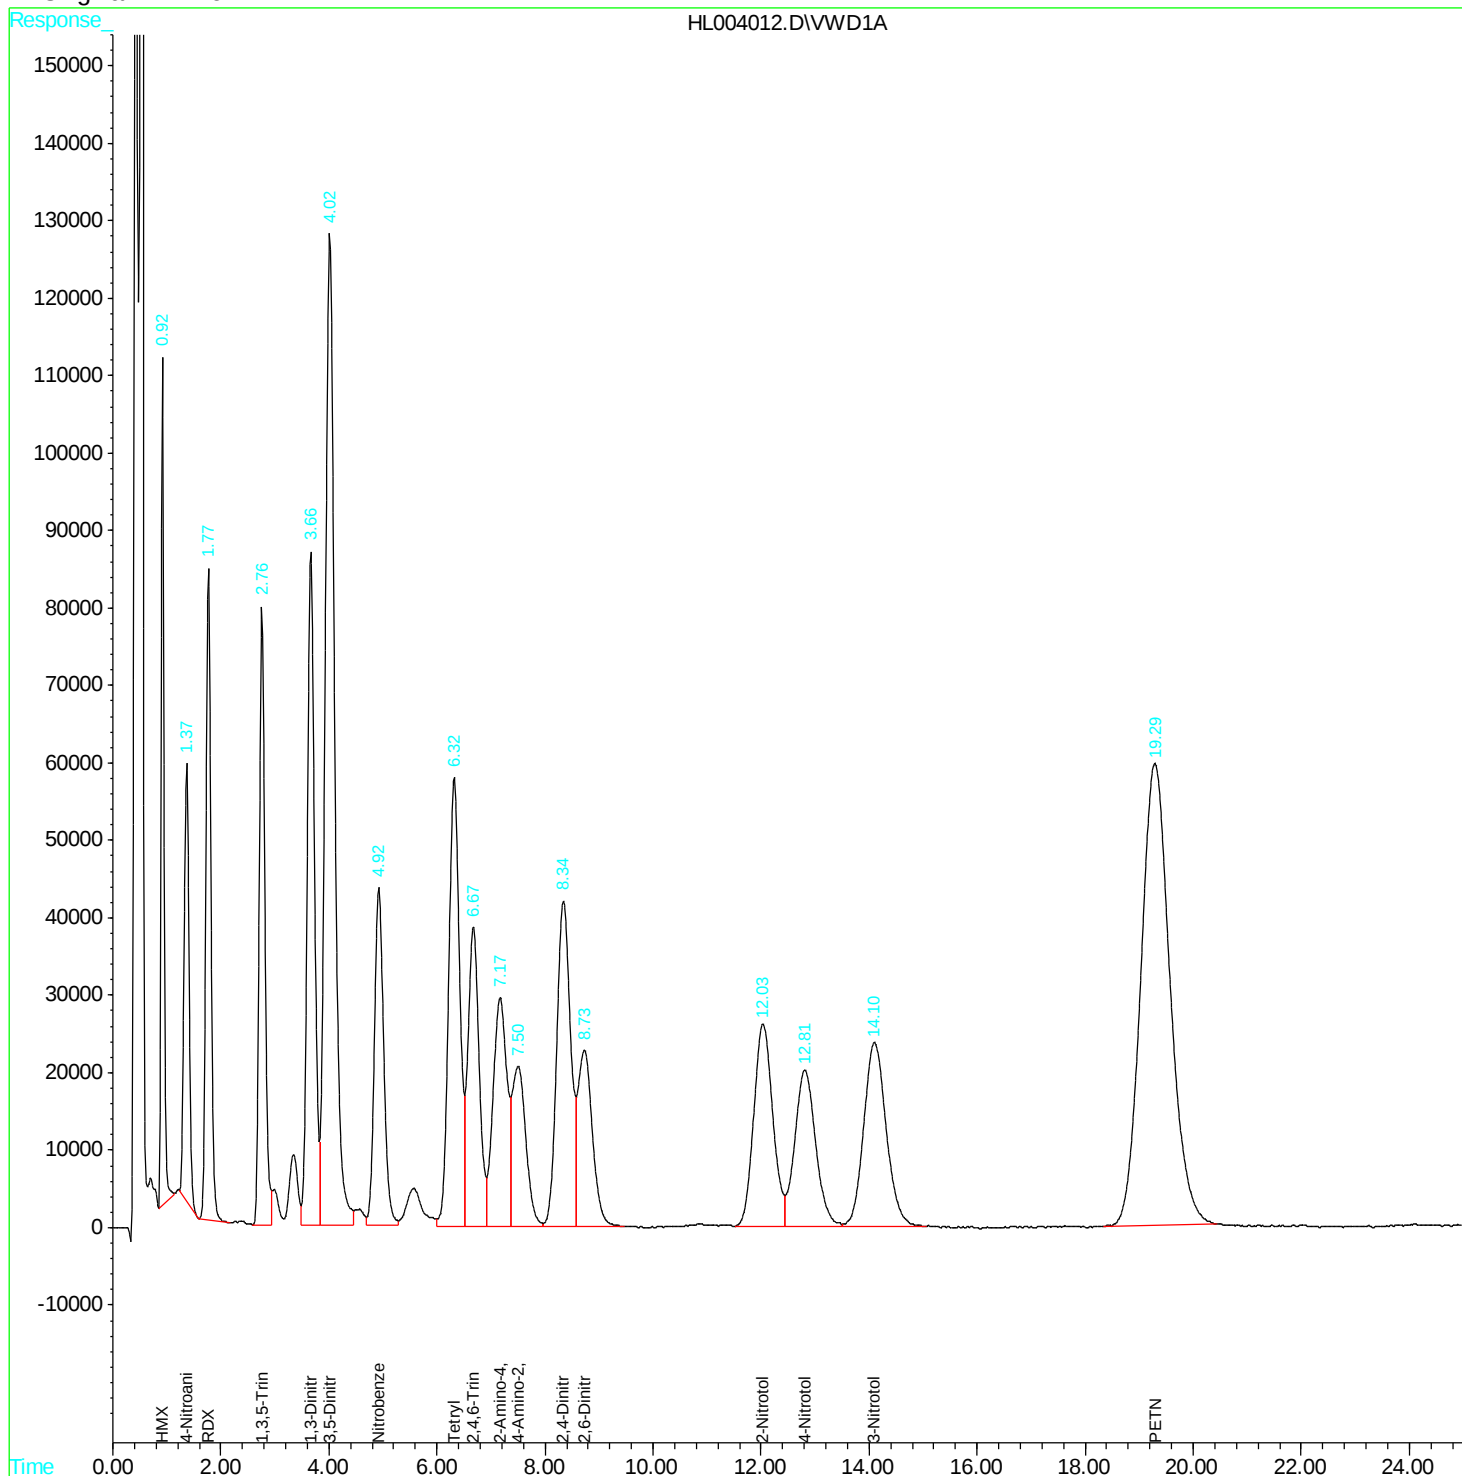


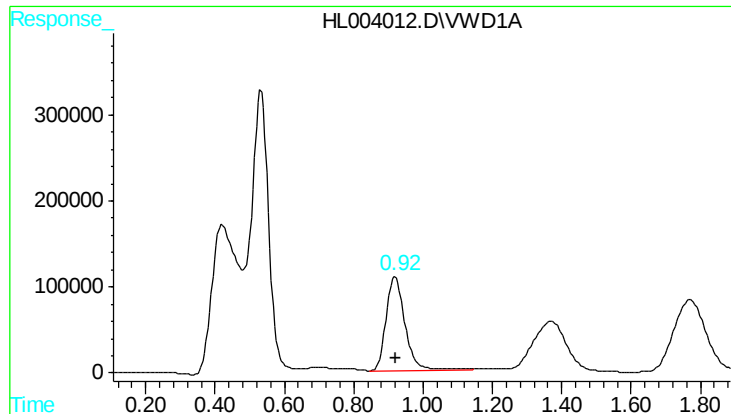

#2 HMX


R.T.: 0.919 min
Delta R.T.: 0.000 min
Response: 4047649
Conc: 941.89 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

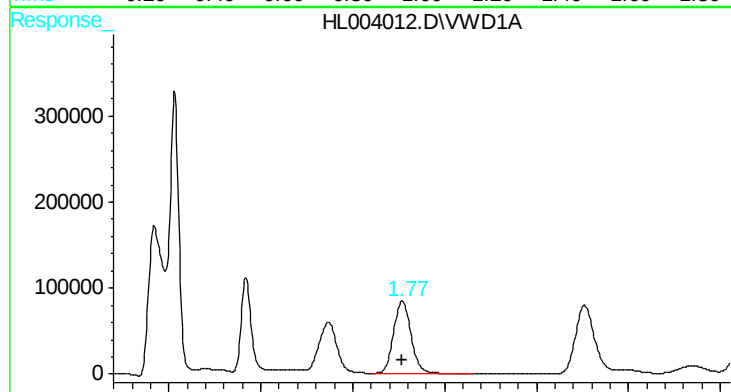


#3 RDX

R.T.: 1.771 min
Delta R.T.: 0.000 min
Response: 5528575
Conc: 1040.94 ug/L

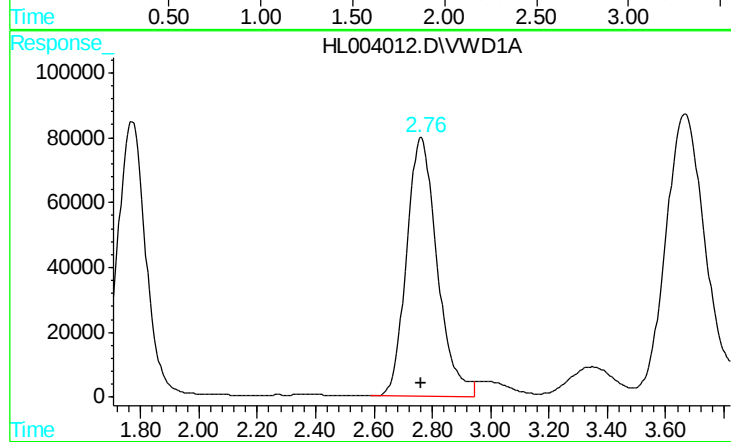


#4 1,3,5-Trinitrobenzene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 5809934
Conc: 492.79 ug/L

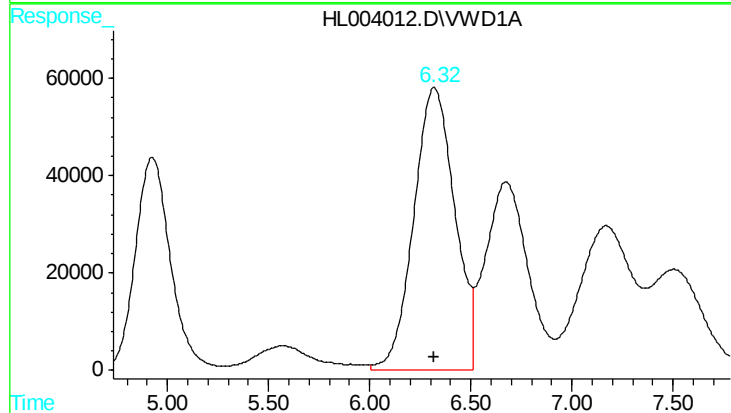

#5 Tetryl


R.T.: 6.320 min
Delta R.T.: 0.003 min
Response: 8193622
Conc: 989.23 ug/L

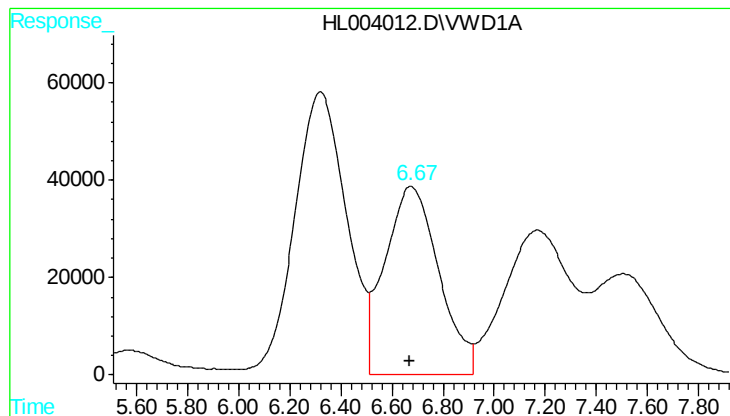

#6 2,4,6-Trinitrotoluene


R.T.: 6.676 min
Delta R.T.: 0.004 min
Response: 5627856
Conc: 504.76 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

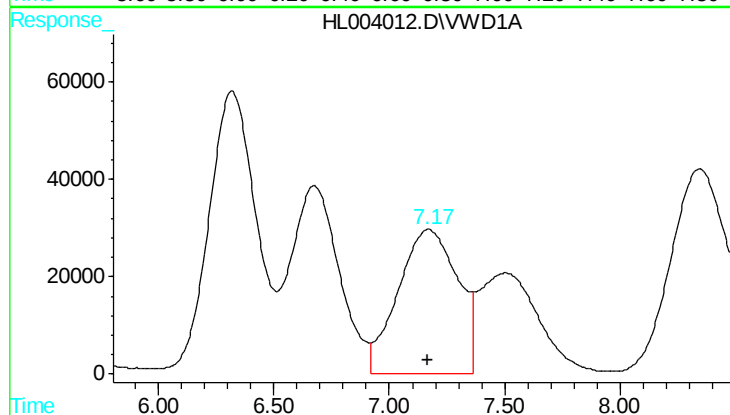


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.170 min
Delta R.T.: 0.004 min
Response: 5324129
Conc: 505.30 ug/L

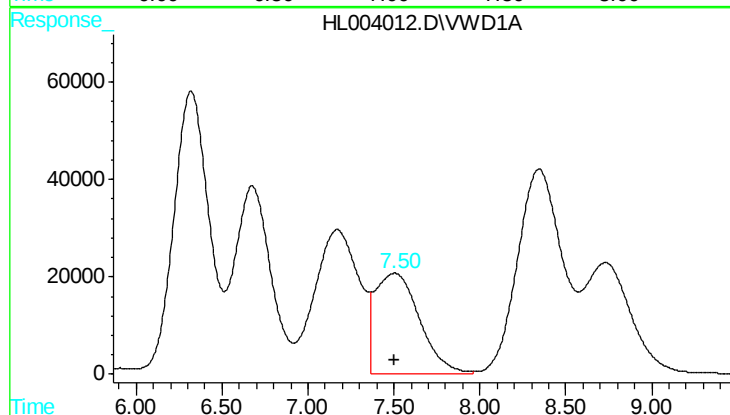


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.504 min
Delta R.T.: 0.000 min
Response: 3696316
Conc: 508.03 ug/L

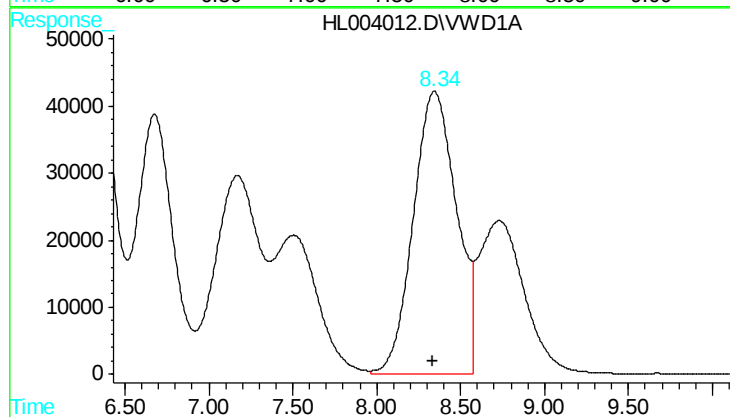

#9 2,4-Dinitrotoluene


R.T.: 8.344 min
Delta R.T.: 0.007 min
Response: 7547602
Conc: 491.17 ug/L

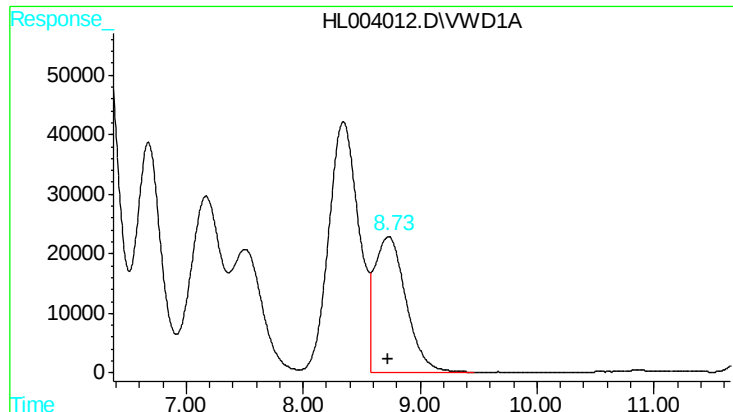

#10 2,6-Dinitrotoluene


R.T.: 8.730 min
Delta R.T.: 0.004 min
Response: 4289993
Conc: 506.86 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

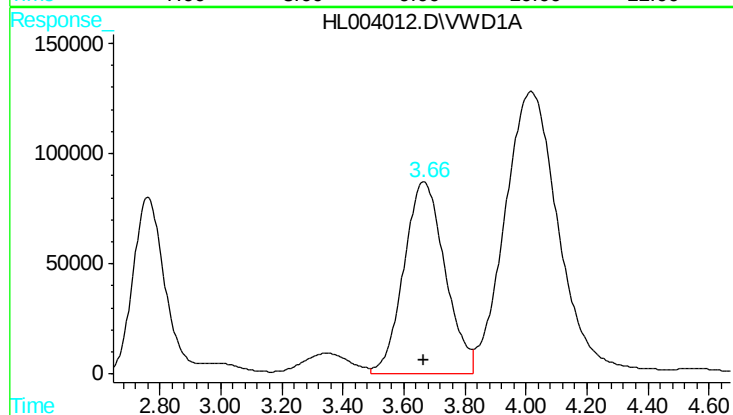


#11 1,3-Dinitrobenzene

R.T.: 3.667 min
Delta R.T.: 0.002 min
Response: 8158968
Conc: 494.20 ug/L

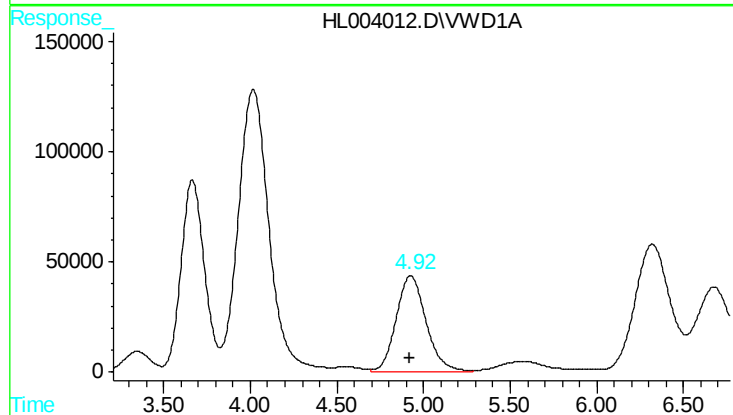


#12 Nitrobenzene

R.T.: 4.926 min
Delta R.T.: 0.005 min
Response: 5251271
Conc: 484.71 ug/L

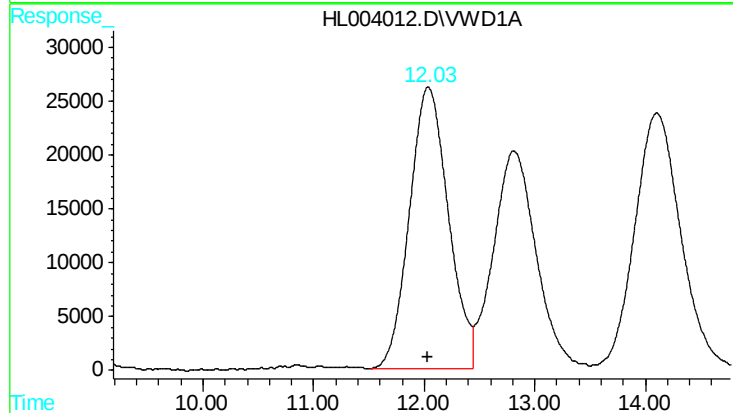

#13 2-Nitrotoluene


R.T.: 12.035 min
Delta R.T.: 0.004 min
Response: 6437122
Conc: 968.19 ug/L

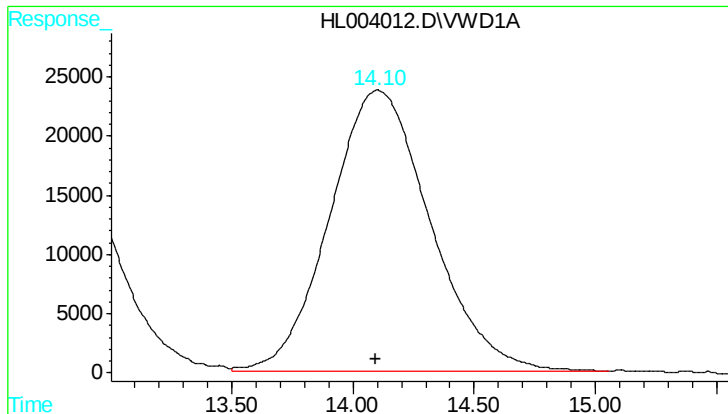

#14 3-Nitrotoluene


R.T.: 14.102 min
Delta R.T.: 0.007 min
Response: 6899086
Conc: 976.48 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

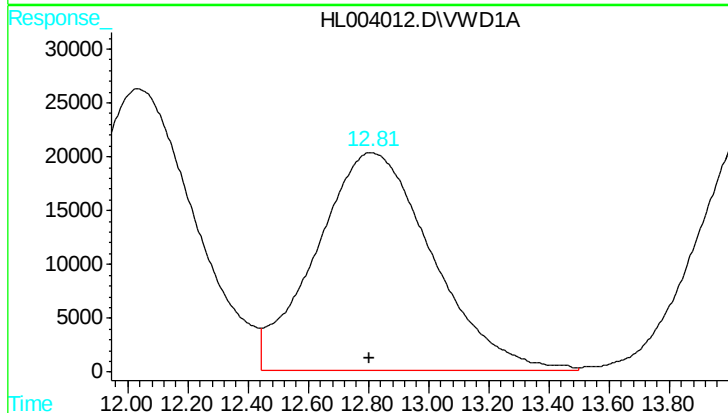


#15 4-Nitrotoluene

R.T.: 12.810 min
Delta R.T.: 0.005 min
Response: 5459798
Conc: 976.61 ug/L

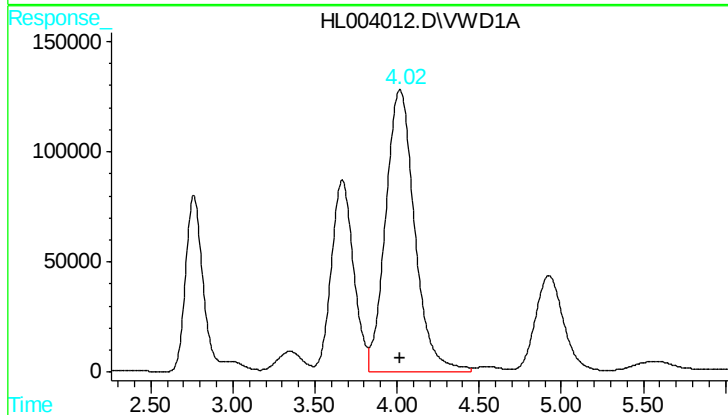

#16 3,5-Dinitroaniline

R.T.: 4.018 min
Delta R.T.: 0.002 min
Response: 15734396
Conc: 980.48 ug/L

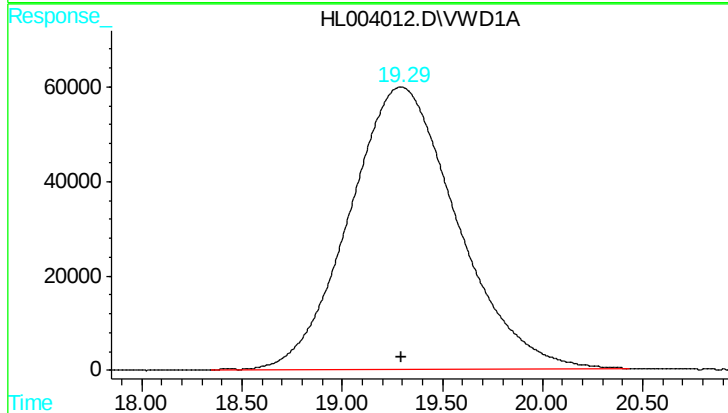

#18 PETN

R.T.: 19.293 min
Delta R.T.: -0.004 min
Response: 22419919
Conc: 2476.40 ug/L