

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010313\
Data File : HL004022.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 08:24
Operator : HLM
Sample : D5191-13
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
MRSSOUTH-ISM-3

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:00:58 AM

Integration File: events.e
Quant Time: Jan 04 22:26:37 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.368	593793	165.103 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	55.03%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010313\
Data File : HL004022.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 08:24
Operator : HLM
Sample : D5191-13
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
MRSSOUTH-ISM-3


Manual Integrations
APPROVED

AHPatel
1/8/2013 3:00:58 AM

Integration File: events.e
Quant Time: Jan 04 22:26:37 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

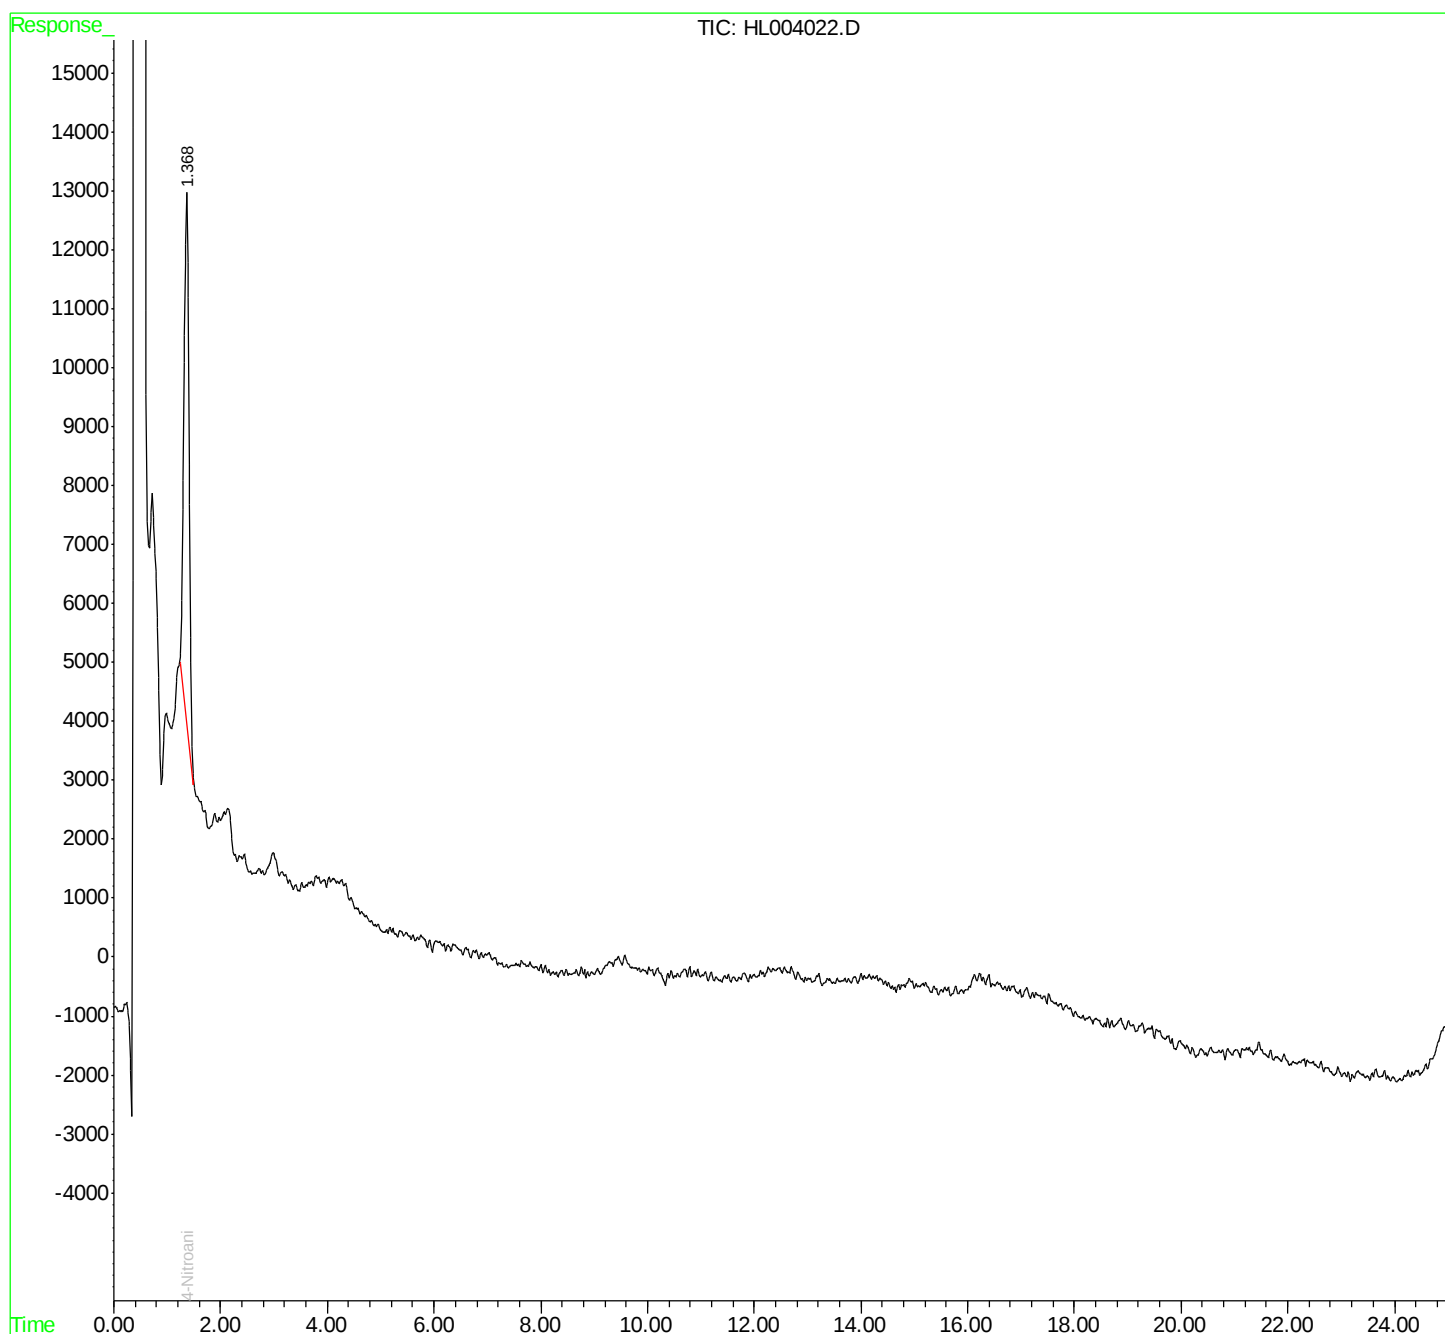

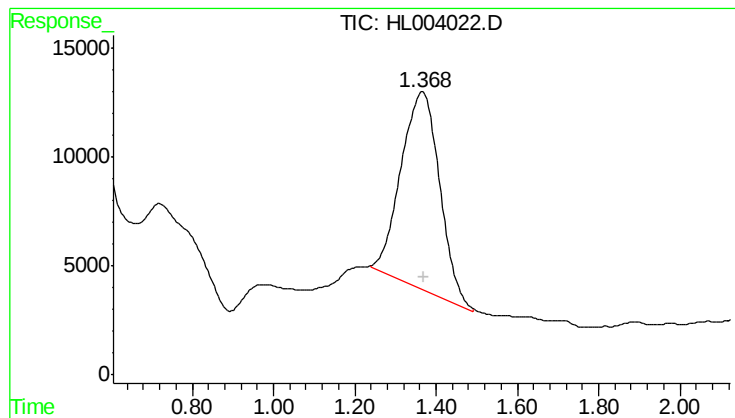

#1 4-Nitroaniline

R.T.: 1.368 min
Delta R.T.: -0.004 min
Response: 593793
Conc: 165.10 ug/L m

Instrument :
HPLC_L
ClientSampleId :
MRSSOUTH-ISM-3

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:00:58 AM