

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010313\
Data File : HL004027.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 10:38
Operator : HLM
Sample : D5191-15
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-3-ISM

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:01:02 AM

Integration File: events.e
Quant Time: Jan 04 22:27:00 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.377	255780	71.119 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	23.71%#
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010313\
Data File : HL004027.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 10:38
Operator : HLM
Sample : D5191-15
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
MRSEAST-3-ISM


Manual Integrations
APPROVED

AHPatel
1/8/2013 3:01:02 AM

Integration File: events.e
Quant Time: Jan 04 22:27:00 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jan 04 13:29:03 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

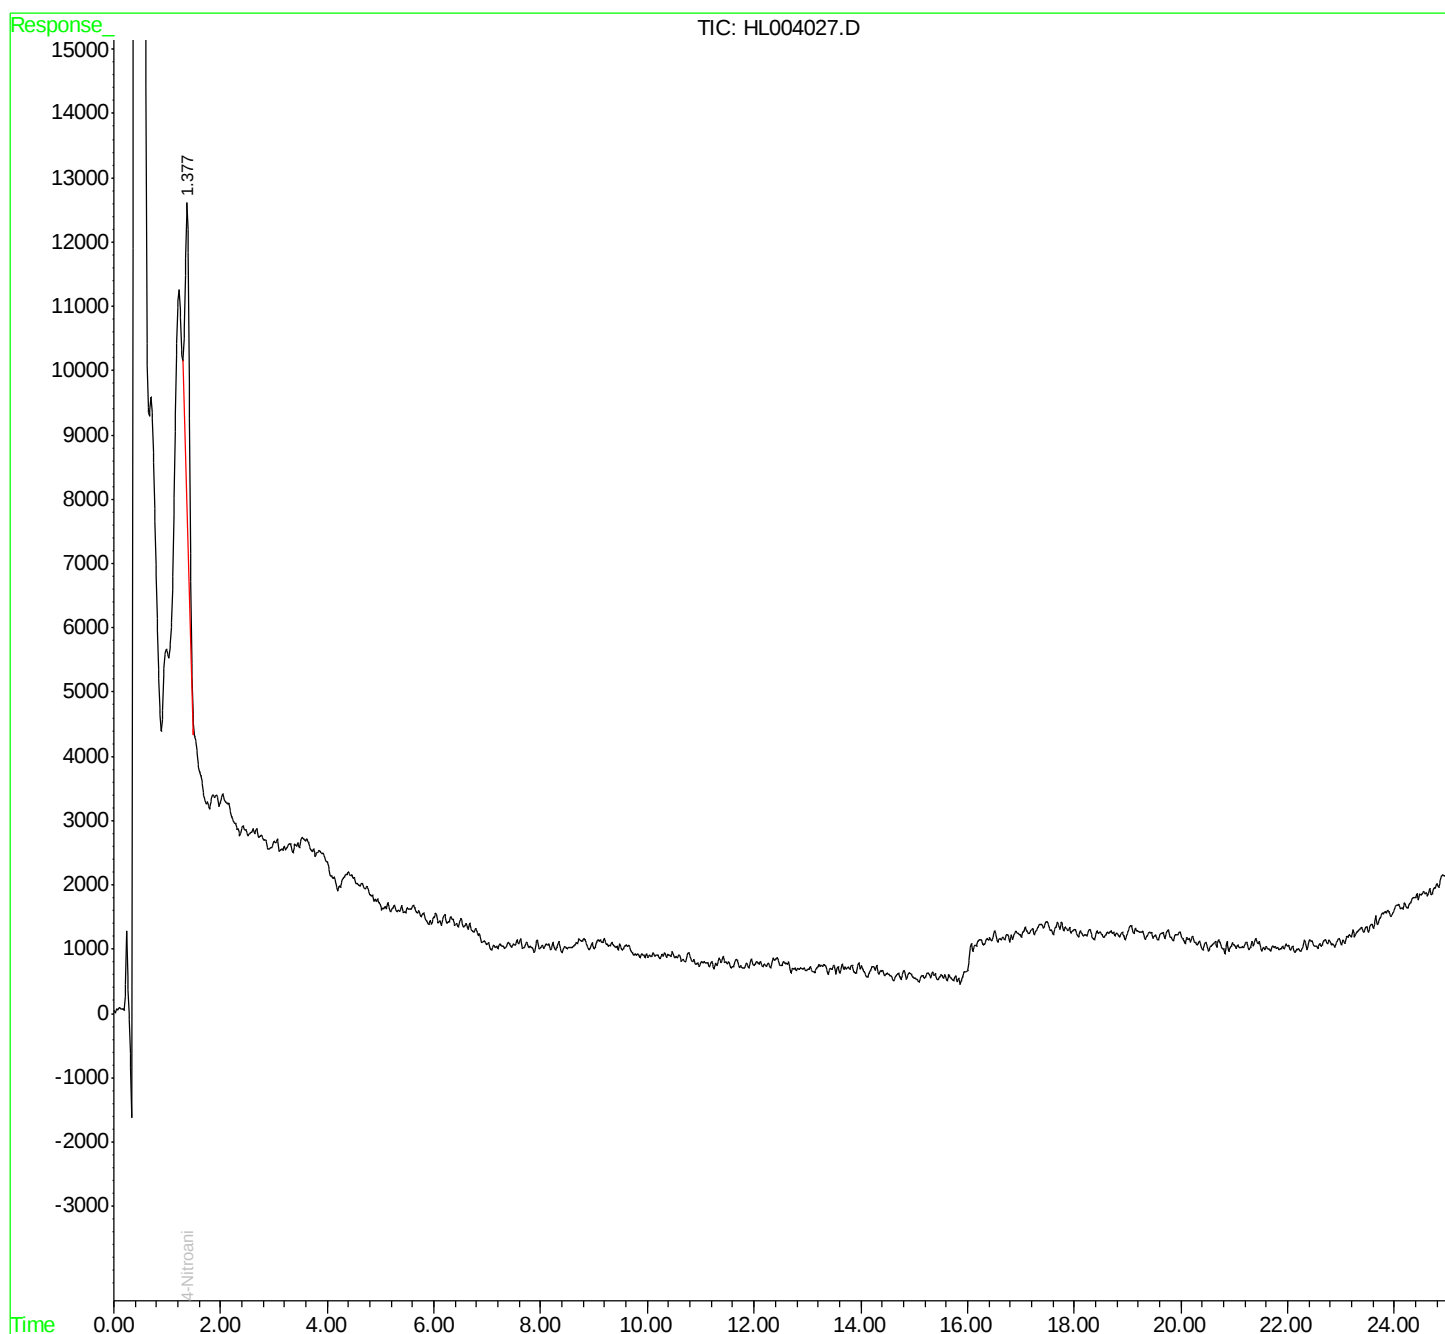

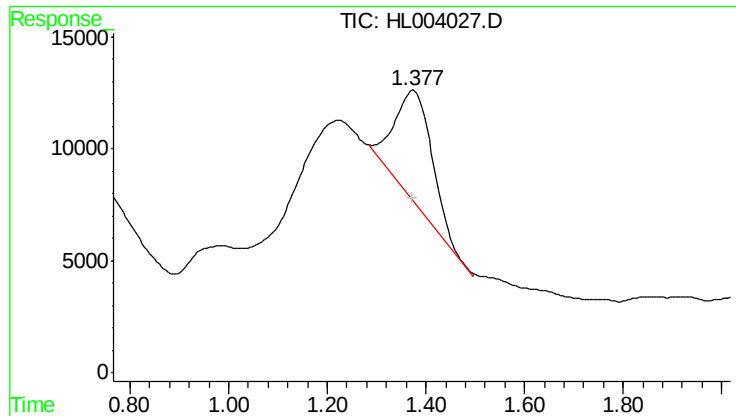

#1 4-Nitroaniline

R.T.: 1.377 min
Delta R.T.: 0.006 min
Response: 255780
Conc: 71.12 ug/L m

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-3-ISM

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:01:02 AM