

Data File : H:\VOL1\HPLC\HPLC L\130104\HL004043.D Vial: 63
Acq On : 04-Jan-2013, 16:24 Operator: HLM
Sample : PB67777BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 7 10:35 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
PB67777BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.38	660433	183.632 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 61.21%

Target Compounds

17) T	Nitroglycerin	6.32f	152922	2667.204 ug/L
-------	---------------	-------	--------	---------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\130104\HL004043.D Vial: 63
 Acq On : 04-Jan-2013, 16:24 Operator: HLM
 Sample : PB67777BS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 7 10:35 2013 Quant Results File: HL010313.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB67777BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Jan 07 10:33:38 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

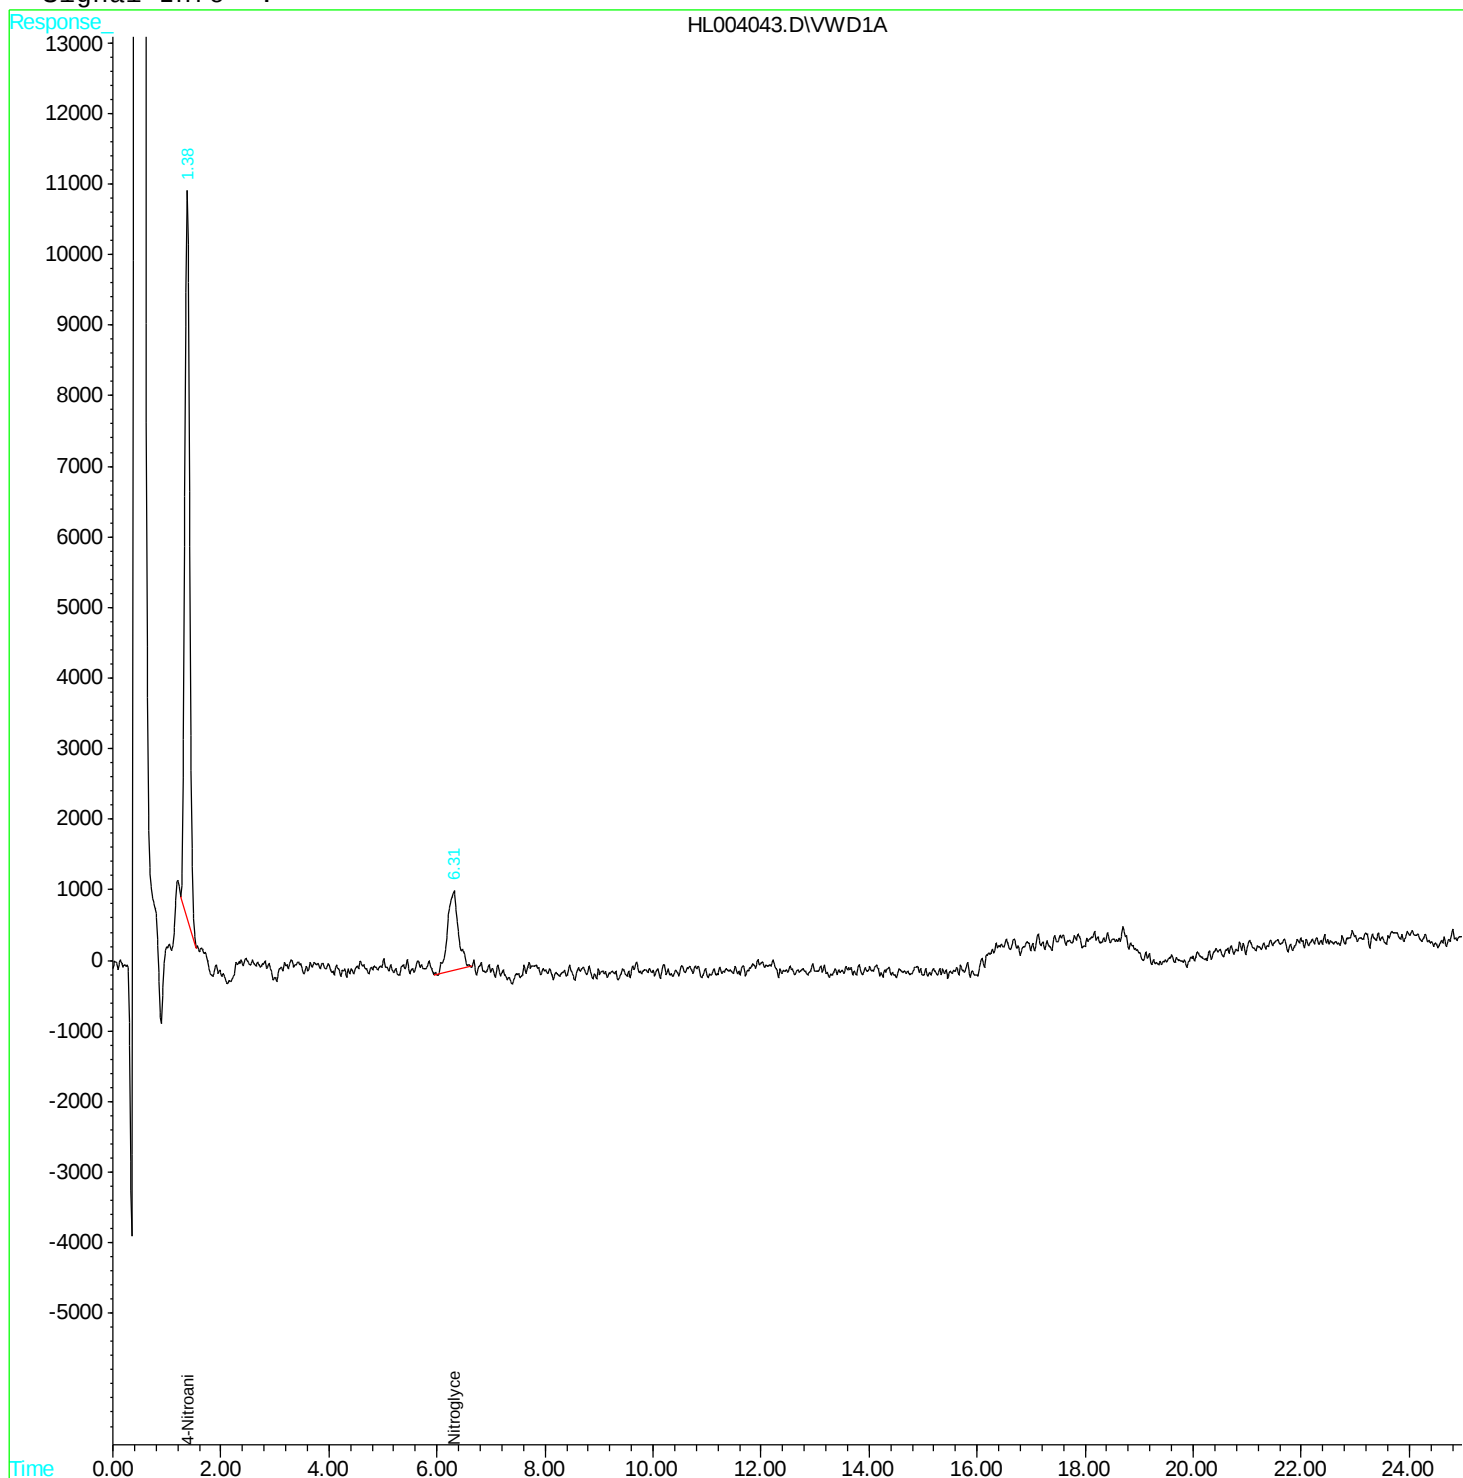

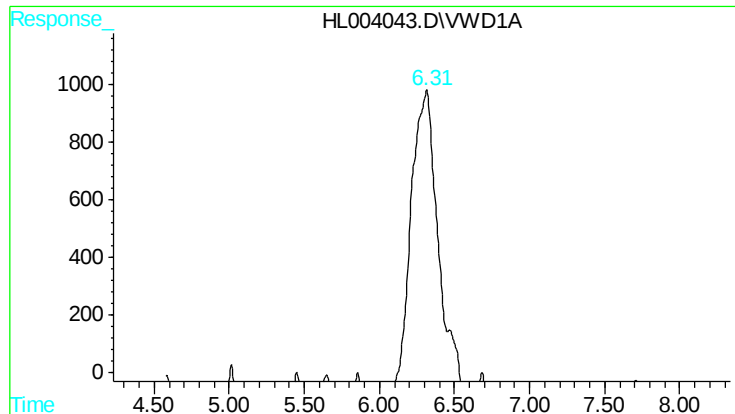

#17 Nitroglycerin

R.T.: 6.316 min
Delta R.T.: 0.045 min
Response: 152922
Conc: 2667.20 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67777BS2