

Data File : H:\VOL1\HPLC\HPLC L\130104\HL004045.D Vial: 65  
 Acq On : 04-Jan-2013, 17:18 Operator: HLM  
 Sample : D5190-11RE Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Jan 7 10:35 2013 Quant Results File: HL010313.RES

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 SAOI4-ISM-1RE

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)  
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
 Last Update : Mon Jan 07 10:33:38 2013  
 Response via : Initial Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. :  
 Signal Phase :  
 Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

#### System Monitoring Compounds

|               |                |       |          |                   |
|---------------|----------------|-------|----------|-------------------|
| 1) S          | 4-Nitroaniline | 1.38  | 575874   | 160.121 ug/L      |
| Spiked Amount | 300.000        | Range | 37 - 149 | Recovery = 53.37% |

#### Target Compounds


|      |                       |       |       |            |
|------|-----------------------|-------|-------|------------|
| 6) T | 2,4,6-Trinitrotoluene | 6.72f | 38925 | 3.491 ug/L |
|------|-----------------------|-------|-------|------------|


Data File : H:\VOL1\HPLC\HPLC L\130104\HL004045.D Vial: 65  
Acq On : 04-Jan-2013, 17:18 Operator: HLM  
Sample : D5190-11RE Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Jan 7 10:35 2013 Quant Results File: HL010313.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
SAOI4-ISM-1RE

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Mon Jan 07 10:33:38 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

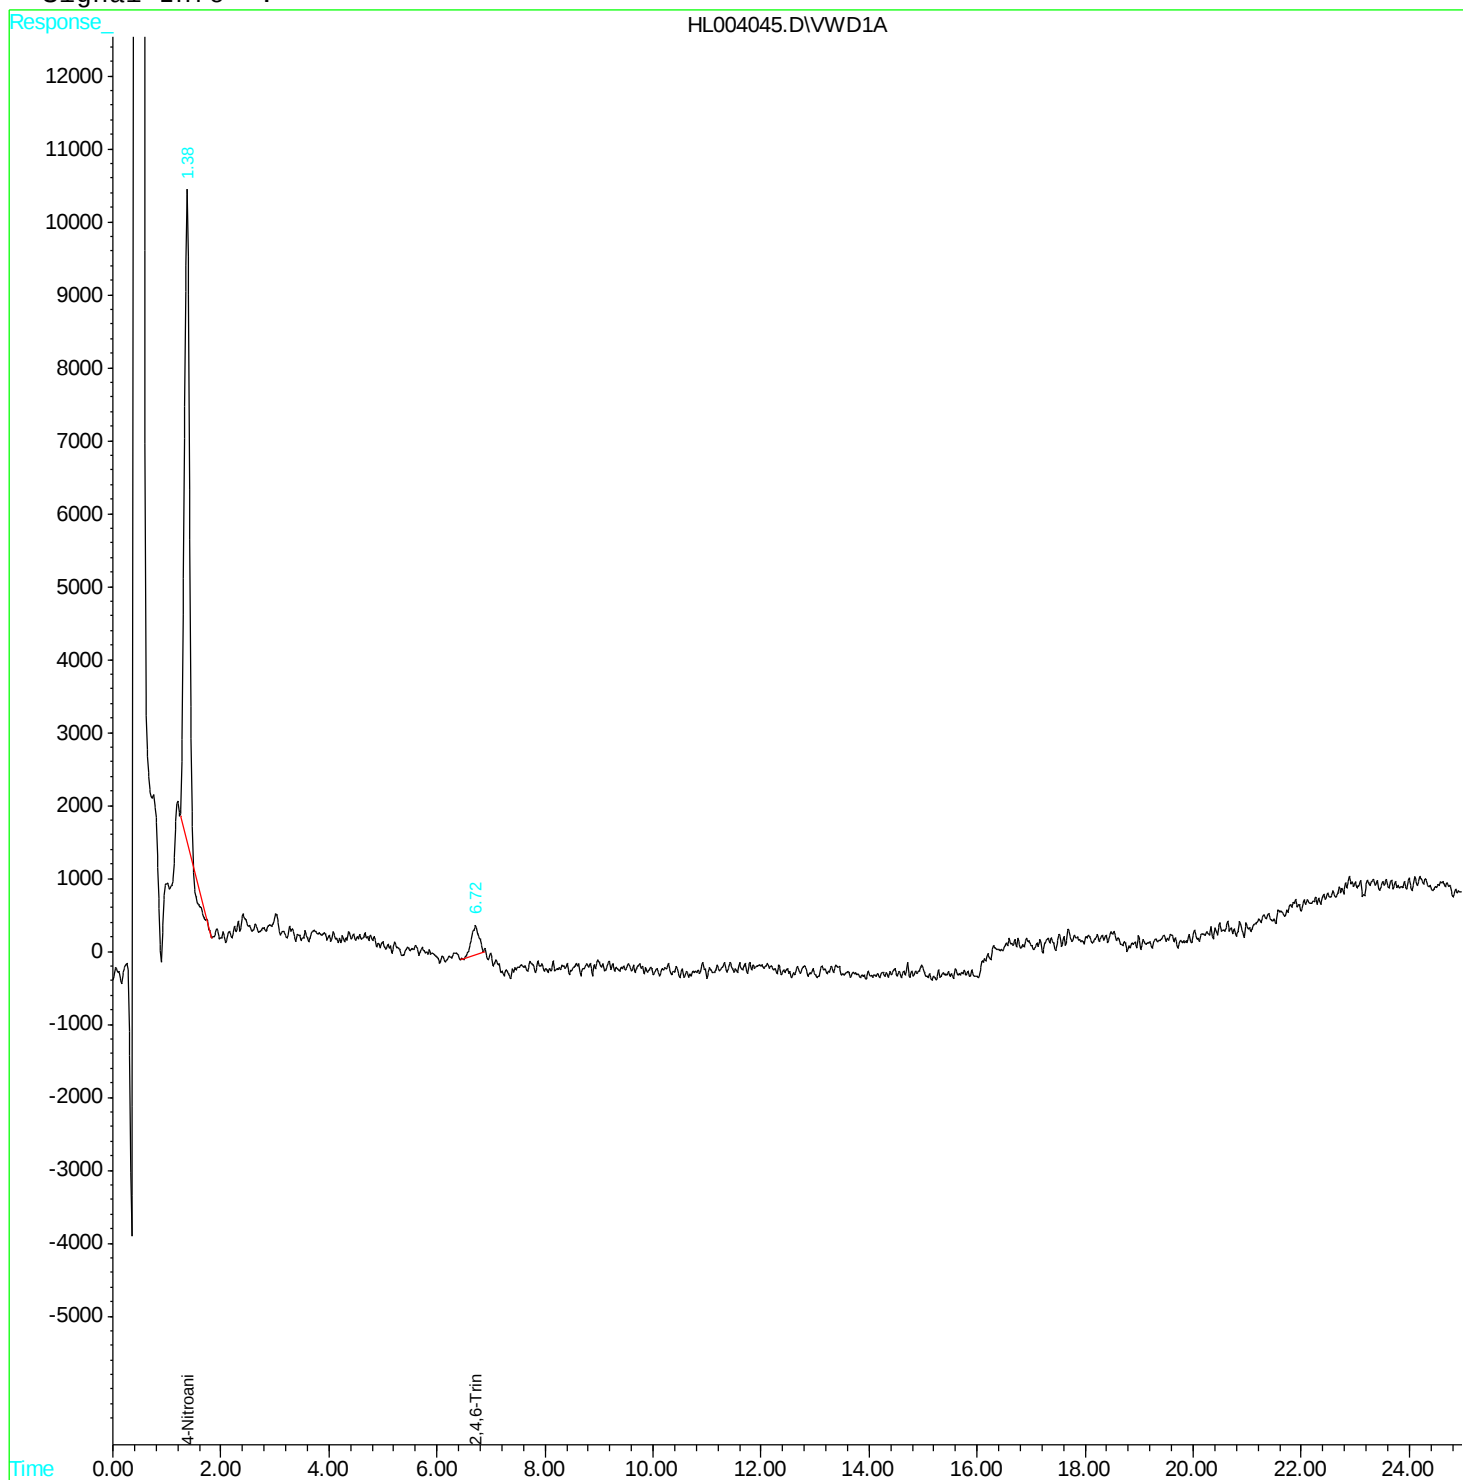

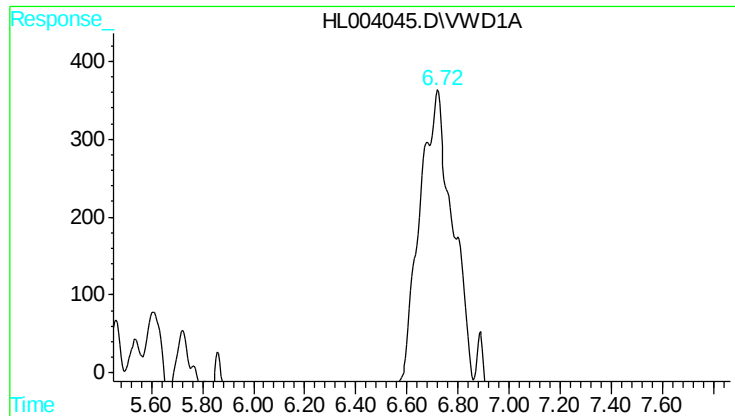

#6 2,4,6-Trinitrotoluene

R.T.: 6.720 min  
Delta R.T.: -0.037 min  
Response: 38925  
Conc: 3.49 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
SAOI4-ISM-1RE