

Data File : H:\VOL1\HPLC\HPLC L\130104\HL004054.D Vial: 75
Acq On : 04-Jan-2013, 21:20 Operator: HLM
Sample : PB67574BSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 7 10:36 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
PB67574BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.38	1189415	330.715 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 110.24%

Target Compounds

17) T	Nitroglycerin	6.29	235478	4107.119 ug/L
-------	---------------	------	--------	---------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\130104\HL004054.D Vial: 75
 Acq On : 04-Jan-2013, 21:20 Operator: HLM
 Sample : PB67574BSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 7 10:36 2013 Quant Results File: HL010313.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB67574BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Jan 07 10:33:38 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

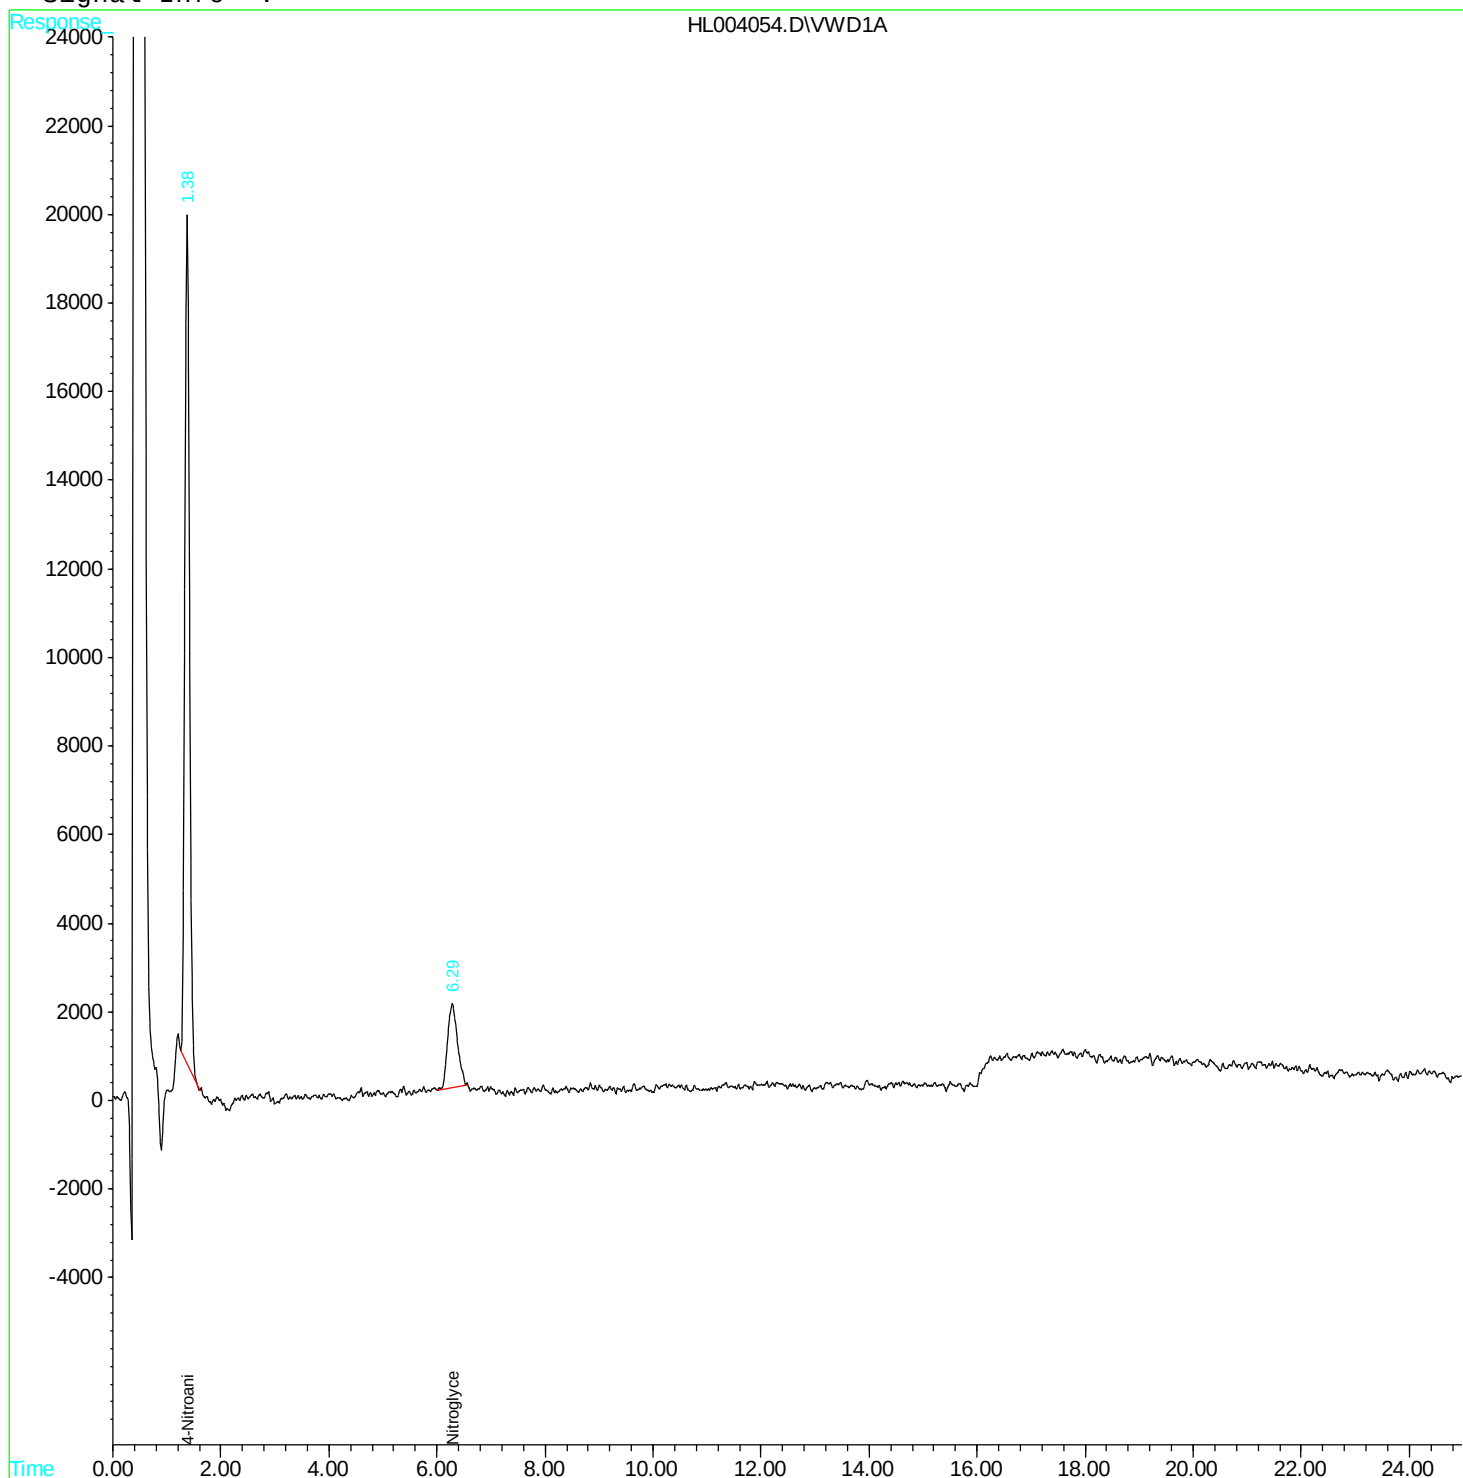

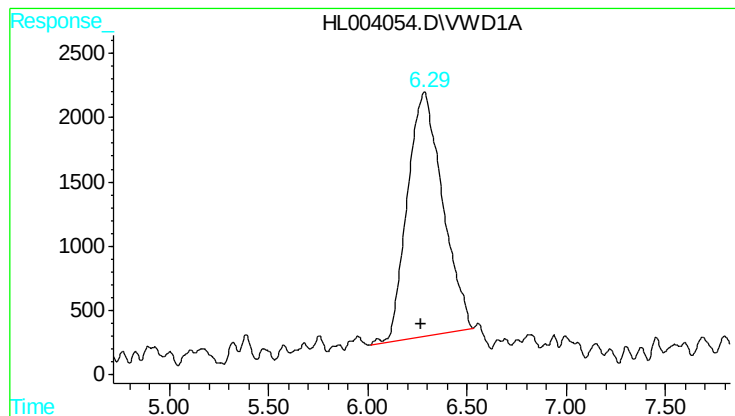

#17 Nitroglycerin

R.T.: 6.288 min
Delta R.T.: 0.017 min
Response: 235478
Conc: 4107.12 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67574BSD2