

Data File : H:\VOL1\HPLC\HPLC L\130104\HL004057.D Vial: 78
Acq On : 04-Jan-2013, 22:41 Operator: HLM
Sample : D5191-10 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 7 10:36 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
QC003-SAOI6

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.38	1818433	505.613 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 168.54%#

Target Compounds


6) T	2,4,6-Trinitrotoluene	6.73	22023	1.975 ug/L
------	-----------------------	------	-------	------------


Data File : H:\VOL1\HPLC\HPLC L\130104\HL004057.D Vial: 78
Acq On : 04-Jan-2013, 22:41 Operator: HLM
Sample : D5191-10 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 7 10:36 2013 Quant Results File: HL010313.RES

Instrument :
HPLC_L
ClientSampleId :
QC003-SAOI6

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL010313.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jan 07 10:33:38 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

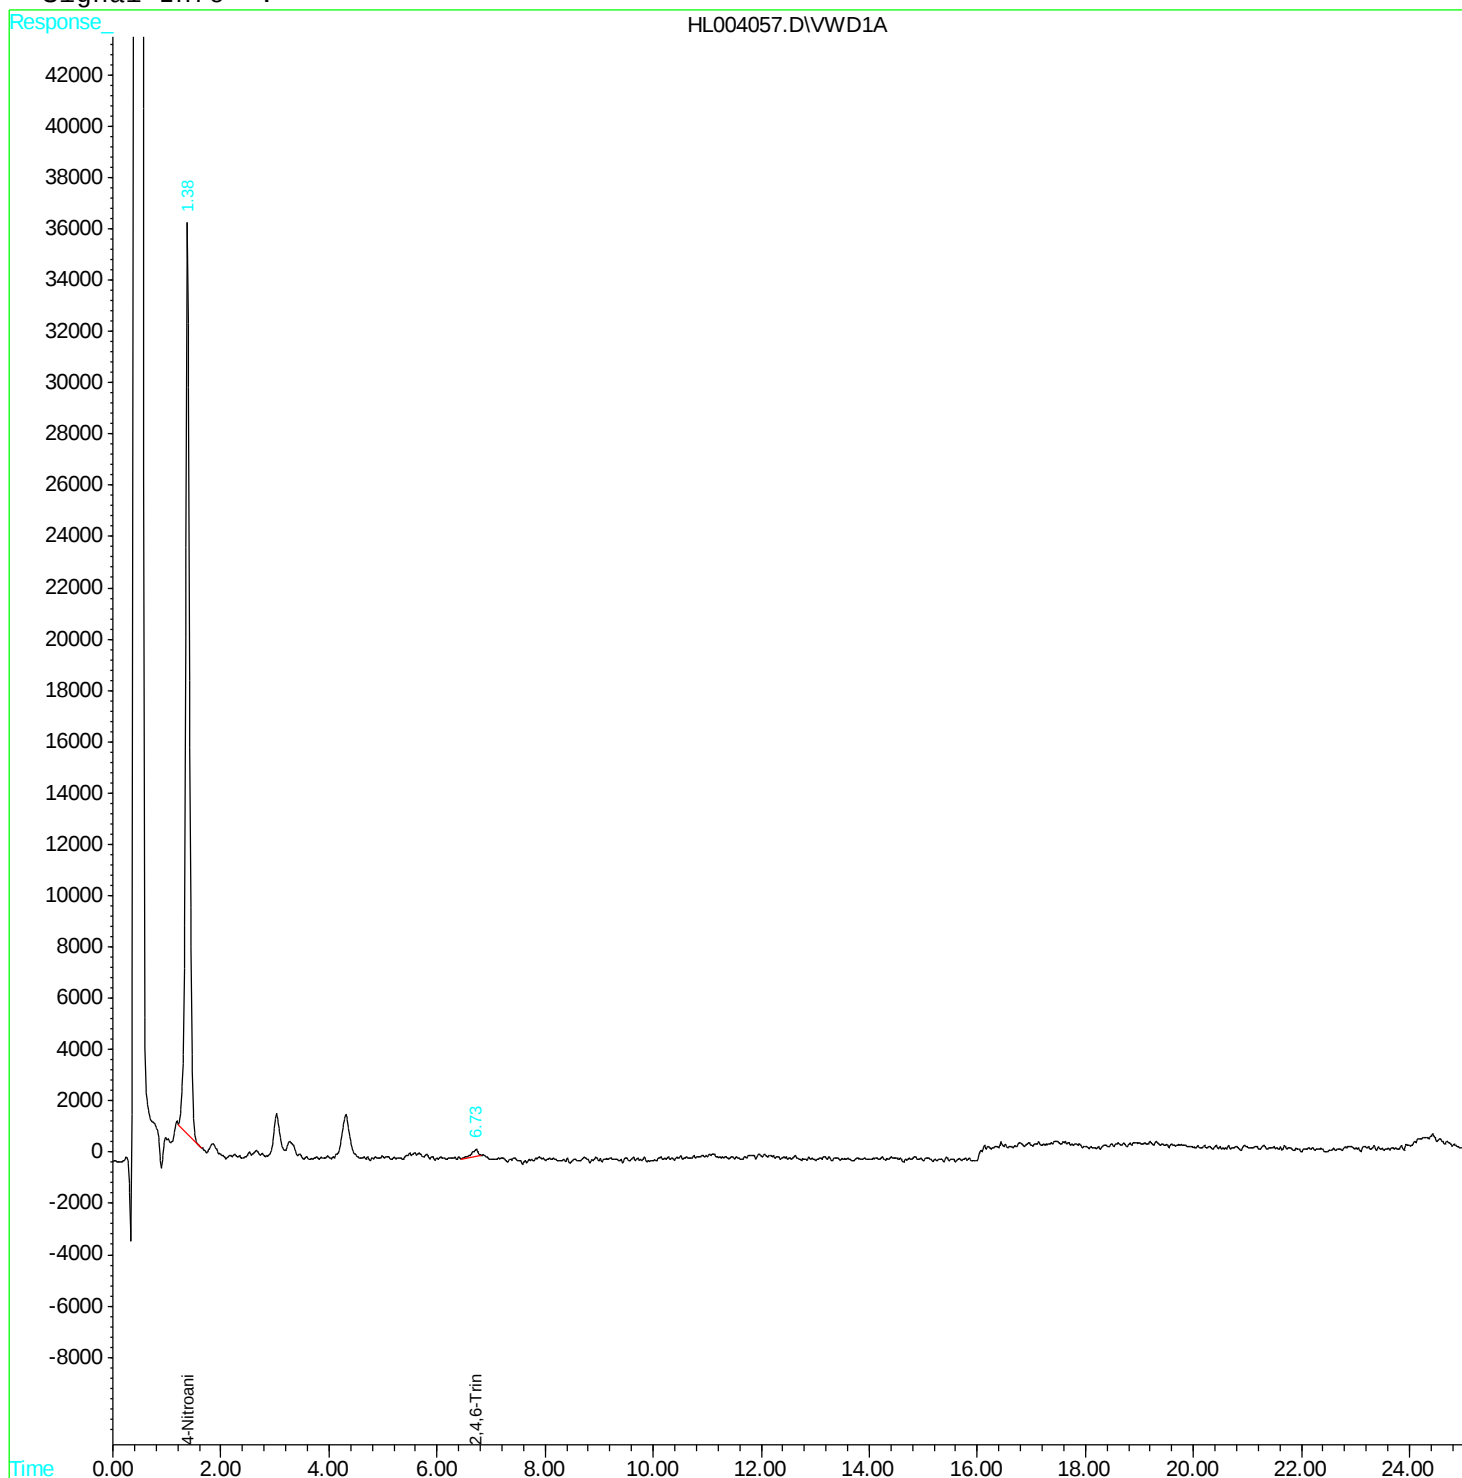

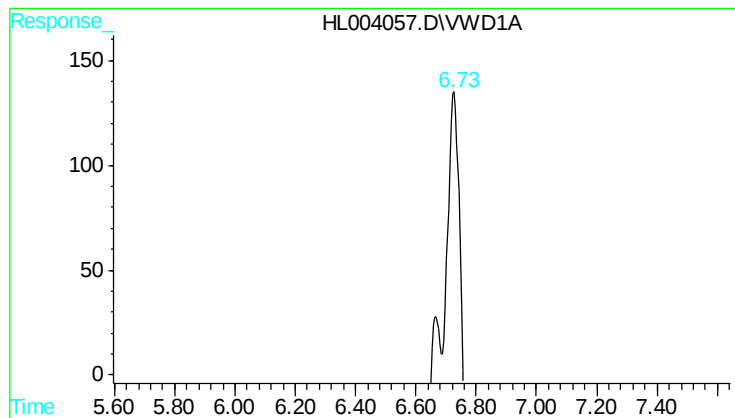

#6 2,4,6-Trinitrotoluene

R.T.: 6.727 min
Delta R.T.: -0.030 min
Response: 22023
Conc: 1.98 ug/L

Instrument :
HPLC_L
ClientSampleId :
QC003-SAOI6