

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010413\
Data File : HL004045.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 17:18
Operator : HLM
Sample : D5190-11RE
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-1RE

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:42 AM

Integration File: events.e
Quant Time: Jan 08 01:26:14 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.378	625439	173.902 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	57.97%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010413\
Data File : HL004045.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 17:18
Operator : HLM
Sample : D5190-11RE
Misc :
ALS Vial : 65 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-1RE


Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:42 AM

Integration File: events.e
Quant Time: Jan 08 01:26:14 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

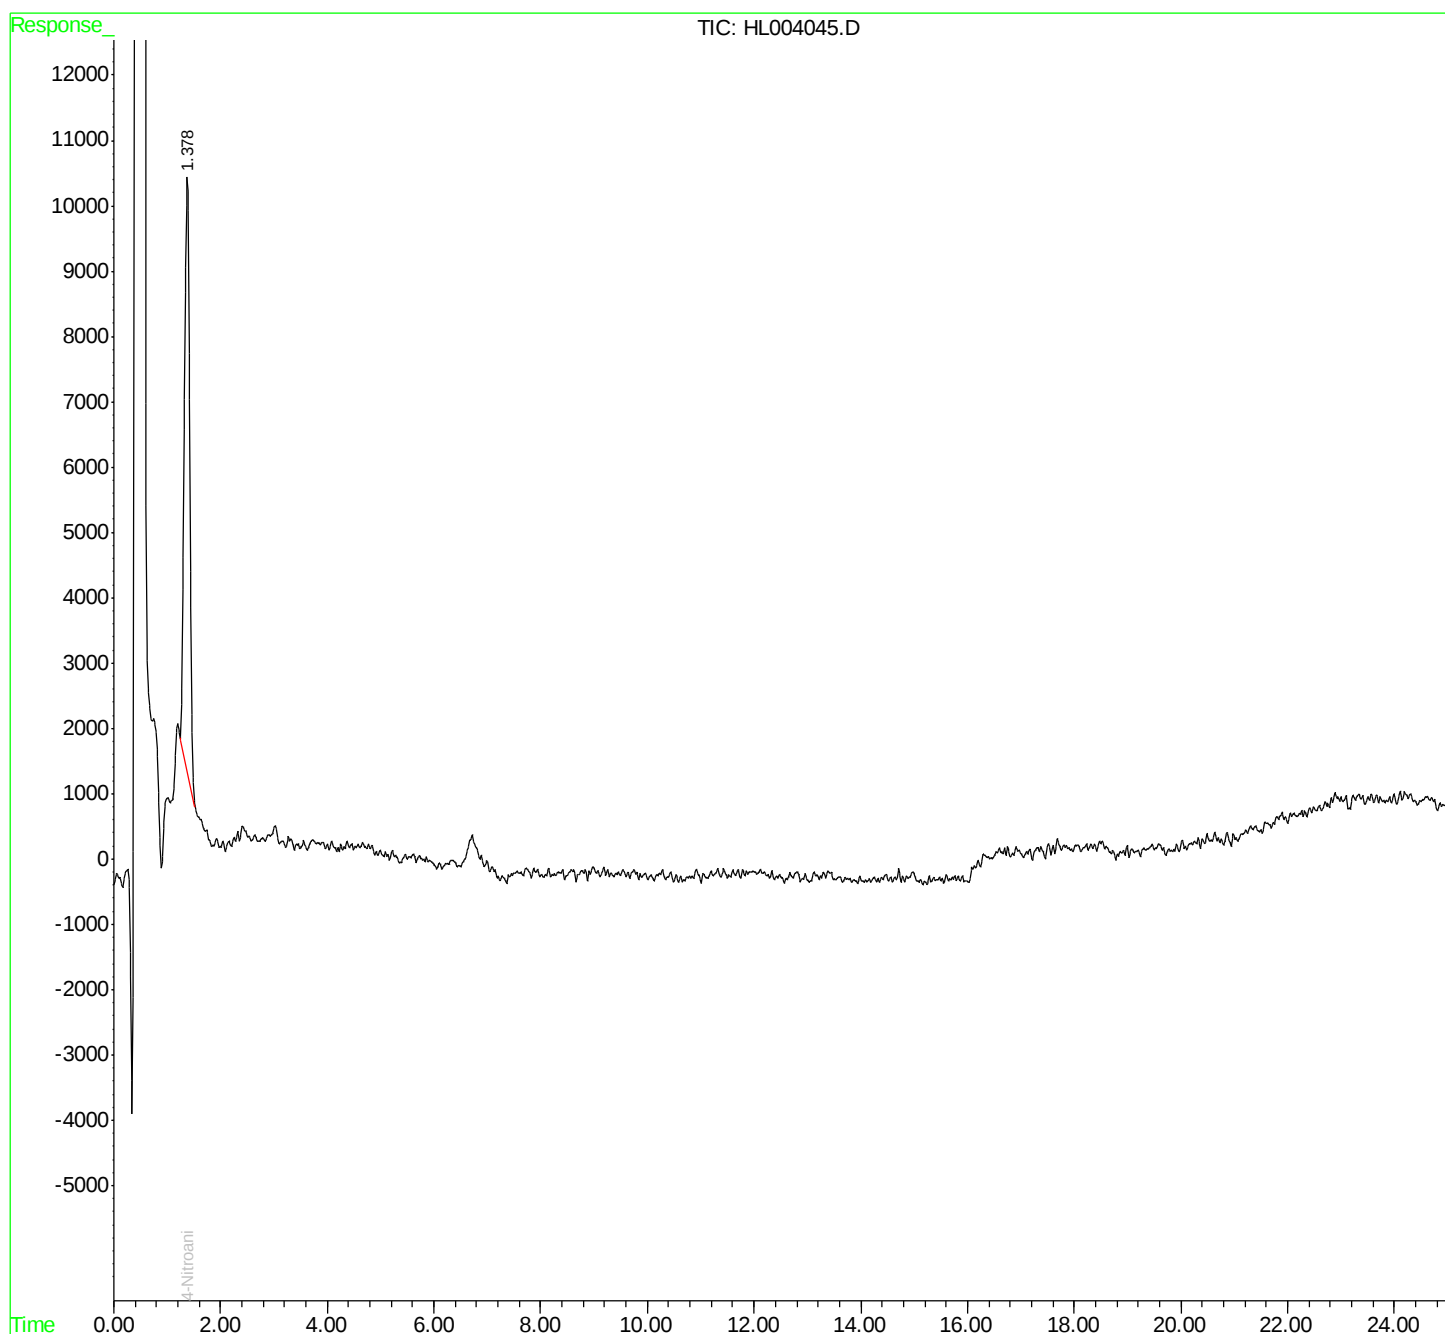

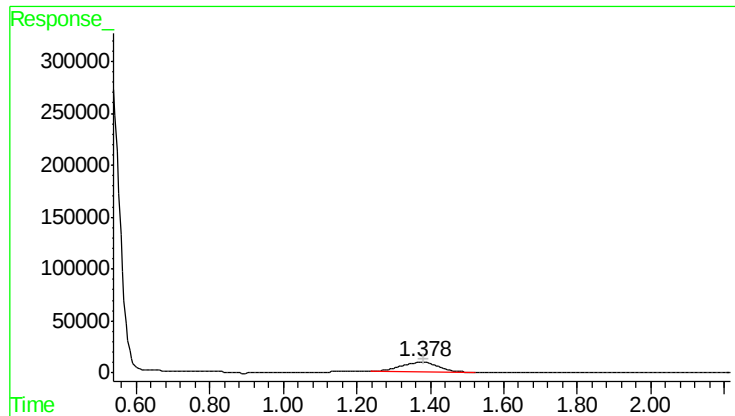

#1 4-Nitroaniline

R.T.: 1.378 min
Delta R.T.: -0.006 min
Response: 625439
Conc: 173.90 ug/L m

Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-1RE

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:42 AM