

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010413\
Data File : HL004046.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 17:45
Operator : HLM
Sample : D5190-14RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1RE

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:44 AM

Integration File: events.e
Quant Time: Jan 08 01:26:19 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.377	625264	173.854 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	57.95%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL010413\
Data File : HL004046.D
Signal(s) : VWD1A.CH
Acq On : 04-Jan-2013, 17:45
Operator : HLM
Sample : D5190-14RE
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1RE


Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:44 AM

Integration File: events.e
Quant Time: Jan 08 01:26:19 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL010313.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Jan 07 10:33:38 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

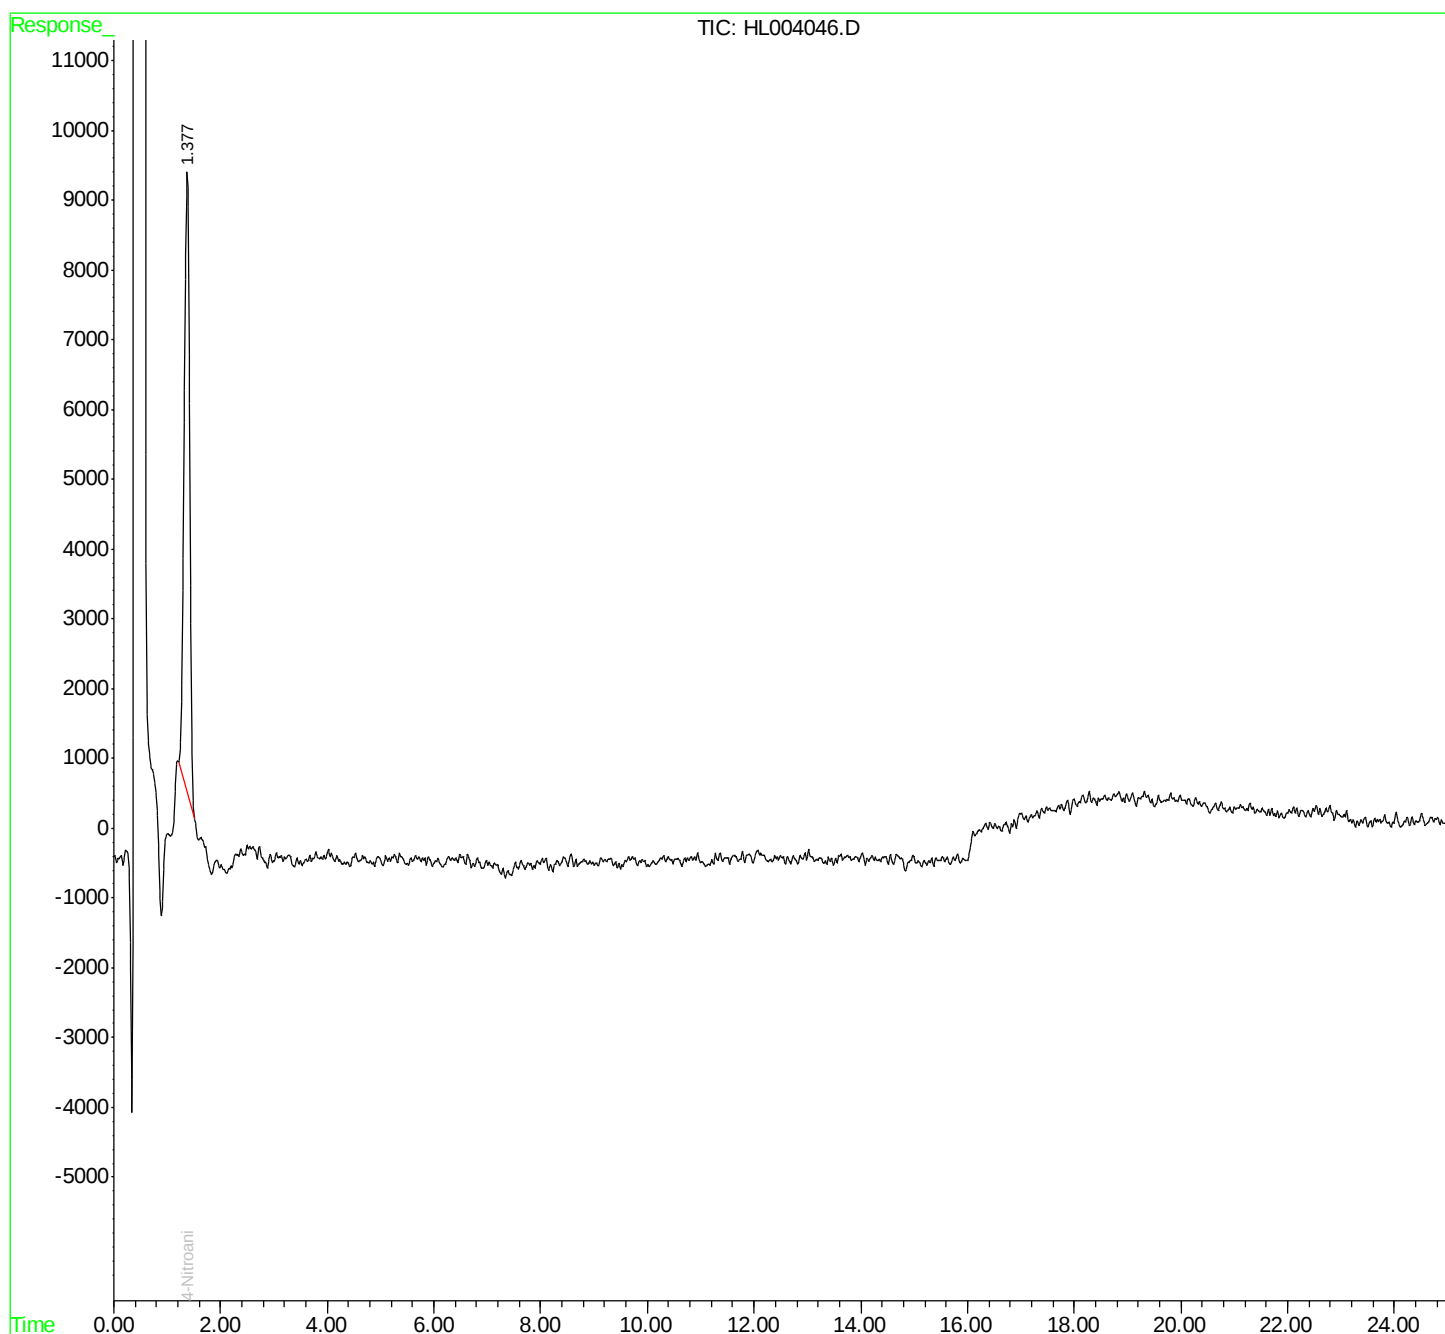

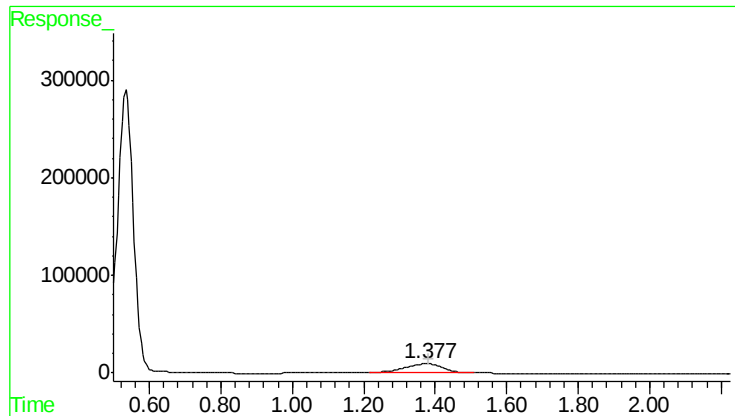

#1 4-Nitroaniline

R.T.: 1.377 min
Delta R.T.: -0.006 min
Response: 625264
Conc: 173.85 ug/L m

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1RE

Manual Integrations
APPROVED

AHPatel
1/8/2013 3:02:44 AM