

Data Path : S:\HPCHEM1\HPLC\_L\Data\HL010413\  
Data File : HL004054.D  
Signal(s) : VWD1A.CH  
Acq On : 04-Jan-2013, 21:20  
Operator : HLM  
Sample : PB67574BSD2  
Misc :  
ALS Vial : 75 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
PB67574BSD2

Manual Integrations  
APPROVED

AHPatel  
1/8/2013 3:02:52 AM

Integration File: events.e  
Quant Time: Jan 08 01:27:07 2013  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL010313.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Mon Jan 07 10:33:38 2013  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound                    | R.T.           | Response | Conc Units      |
|-----------------------------|----------------|----------|-----------------|
| -----                       |                |          |                 |
| System Monitoring Compounds |                |          |                 |
| 1) S 4-Nitroaniline         | 1.379          | 1189415  | 330.715 ug/L    |
| Spiked Amount 300.000       | Range 37 - 149 | Recovery | = 110.24%       |
|                             |                |          |                 |
| Target Compounds            |                |          |                 |
| 17) T Nitroglycerin         | 6.286          | 248128   | 4327.752 ug/L m |
| -----                       |                |          |                 |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : S:\HPCHEM1\HPLC\_L\Data\HL010413\  
Data File : HL004054.D  
Signal(s) : VWD1A.CH  
Acq On : 04-Jan-2013, 21:20  
Operator : HLM  
Sample : PB67574BSD2  
Misc :  
ALS Vial : 75 Sample Multiplier: 1


Instrument :  
HPLC\_L  
ClientSampleId :  
PB67574BSD2


Manual Integrations  
APPROVED

AHPatel  
1/8/2013 3:02:52 AM

Integration File: events.e  
Quant Time: Jan 08 01:27:07 2013  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL010313.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Mon Jan 07 10:33:38 2013  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

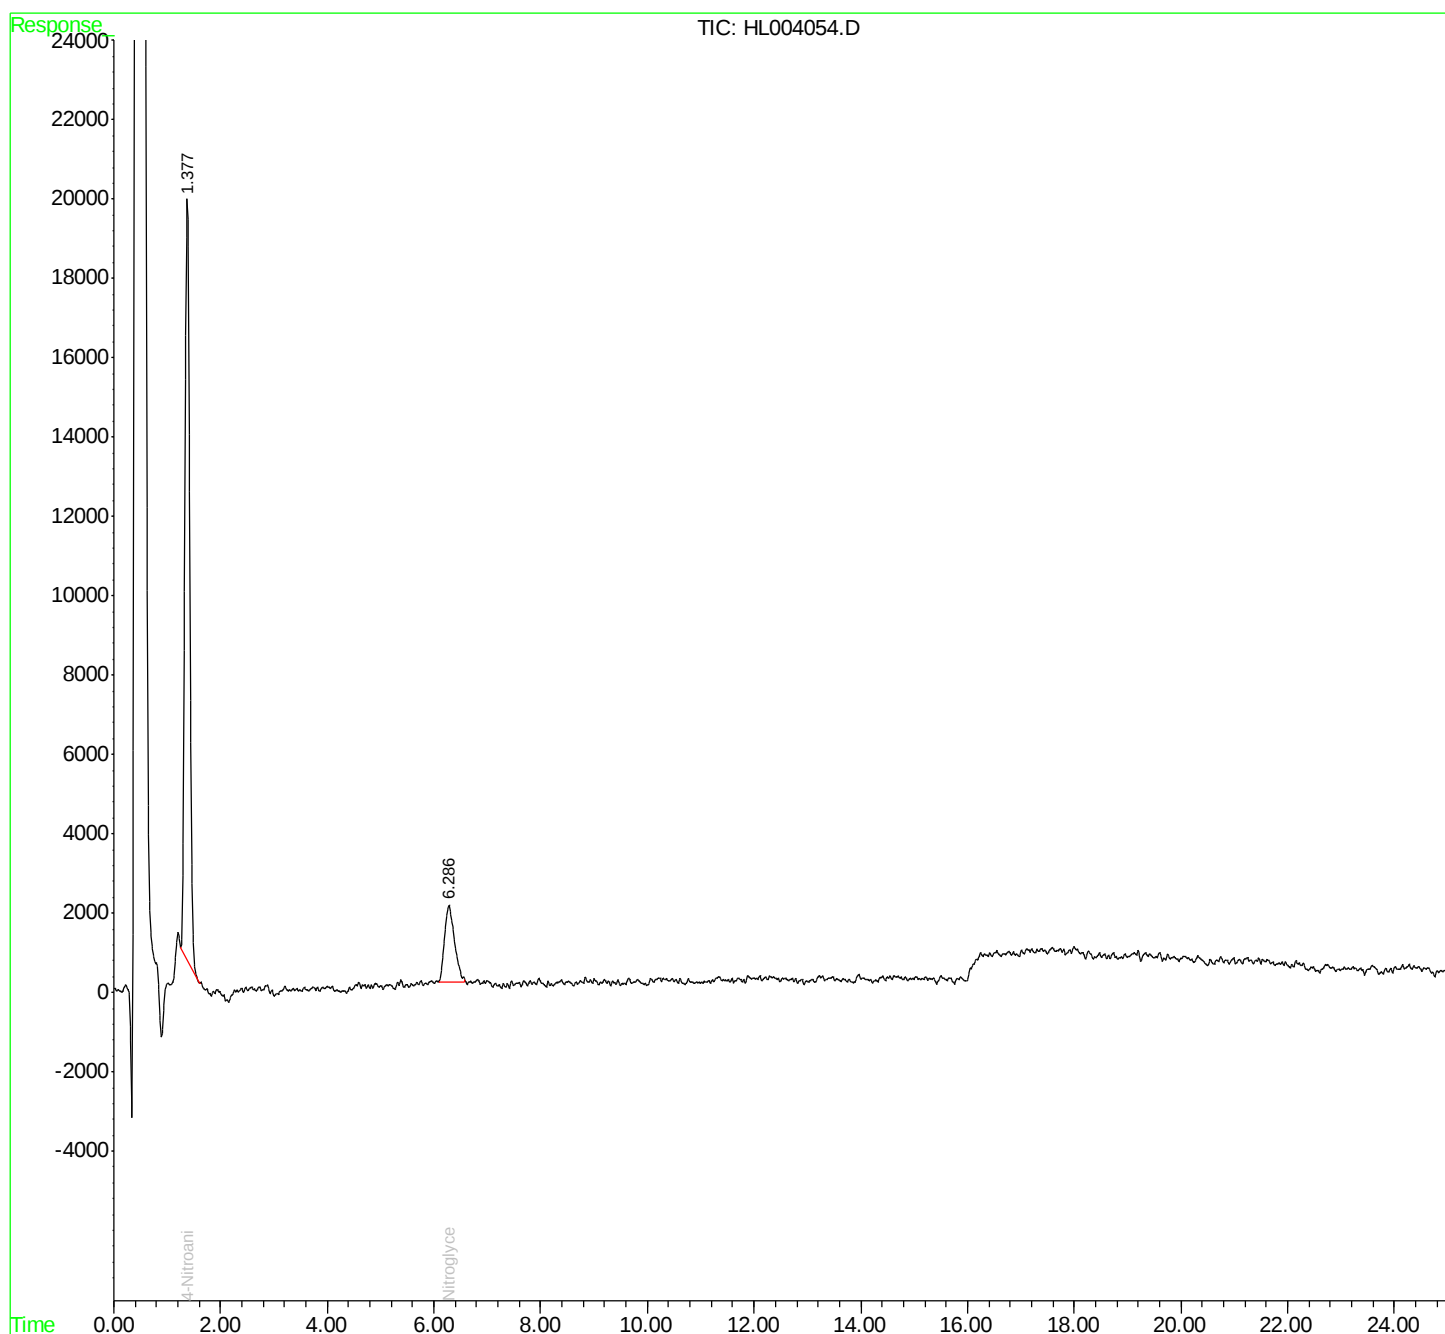

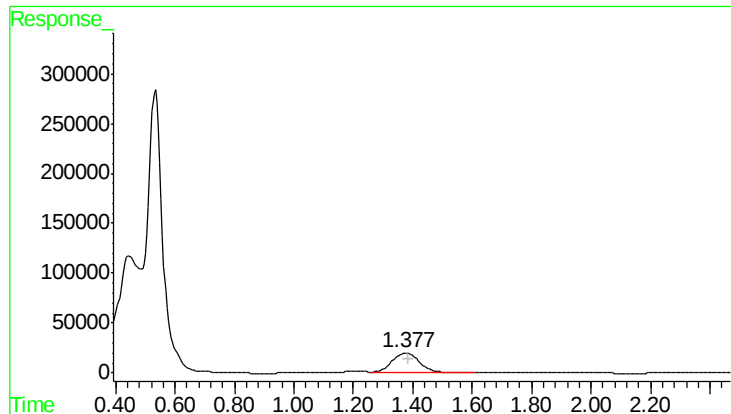


#1 4-Nitroaniline

R.T.: 1.379 min  
Delta R.T.: -0.004 min  
Response: 1189415  
Conc: 330.72 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
PB67574BSD2

Manual Integrations  
APPROVED

AHPatel  
1/8/2013 3:02:52 AM

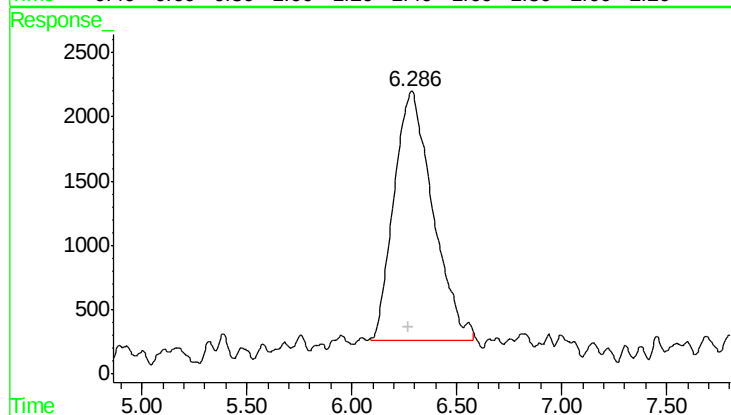

#17 Nitroglycerin

R.T.: 6.286 min  
Delta R.T.: 0.015 min  
Response: 248128  
Conc: 4327.75 ug/L m