

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL020613\HL005019.D Vial: 18
Acq On : 06-Feb-2013, 19:28 Operator: QM
Sample : MDL-S-BLK Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 7 12:04 2013 Quant Results File: HL020613.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL020613.M
Title :
Last Update : Thu Feb 07 11:25:51 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds


Target Compounds


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL020613\HL005019.D Vial: 18
Acq On : 06-Feb-2013, 19:28 Operator: QM
Sample : MDL-S-BLK Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 7 12:04 2013 Quant Results File: HL020613.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL020613.M
Title :
Last Update : Thu Feb 07 11:25:51 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

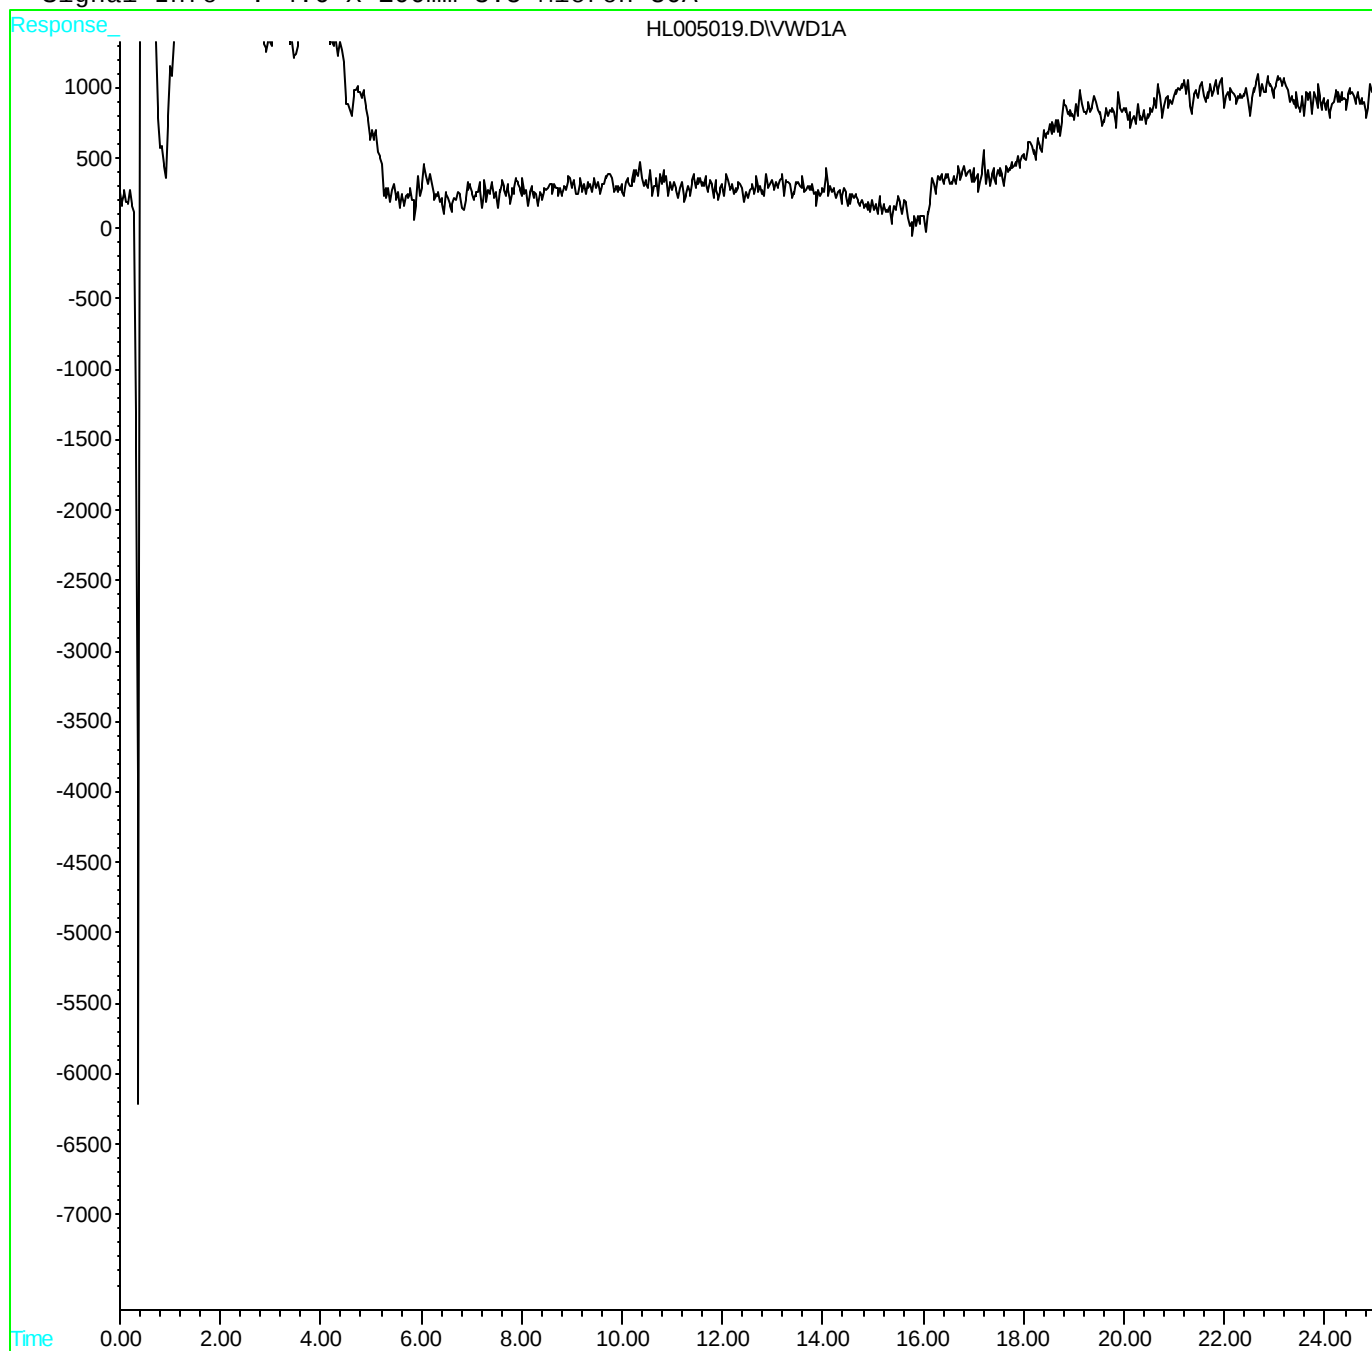

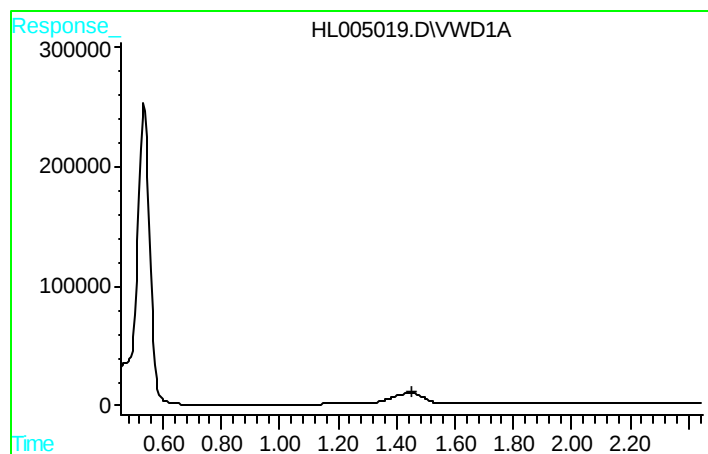

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 1.454 min
Response: 0
Conc: N.D.