

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL032213\
 Data File : HL005165.D
 Signal(s) : VWD1A.CH
 Acq On : 22-Mar-2013, 11:09
 Operator : QM
 Sample : HTSDCCC0500
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 HTSDCCC0500

Integration File: autoint1.e
 Quant Time: Mar 26 03:50:50 2013
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL032013.M
 Quant Title :
 QLast Update : Mon Mar 11 14:17:48 2013
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.404	2202659	494.999 ug/L
Target Compounds			
2) T HMX	0.938	2577783	550.579 ug/L
3) T RDX	1.831	2780752	521.108 ug/L
4) T 1,3,5-Trinitrobenzene	2.841	6011252	511.688 ug/L
5) T 3,5-Dinitroaniline	3.766	8400770	498.663 ng/ml
6) T 1,3-Dinitrobenzene	4.128	6955027	491.483 ug/L
7) T Nitrobenzene	5.043	5398733	512.731 ug/L
8) T Tetryl	6.561	4230786	548.000 ug/L
9) T 2,4,6-Trinitrotoluene	6.880	6200828	514.145 ug/L
10) T 2-Amino-4,6-dinitroto...	7.416	5890644	481.213 ug/L
11) T 4-Amino-2,6-dinitroto...	7.810	3593096	551.742 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL032213\
Data File : HL005165.D
Signal(s) : VWD1A.CH
Acq On : 22-Mar-2013, 11:09
Operator : QM
Sample : HTSDCCC0500
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
HTSDCCC0500

Integration File: autoint1.e
Quant Time: Mar 26 03:50:50 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL032013.M
Quant Title :
QLast Update : Mon Mar 11 14:17:48 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

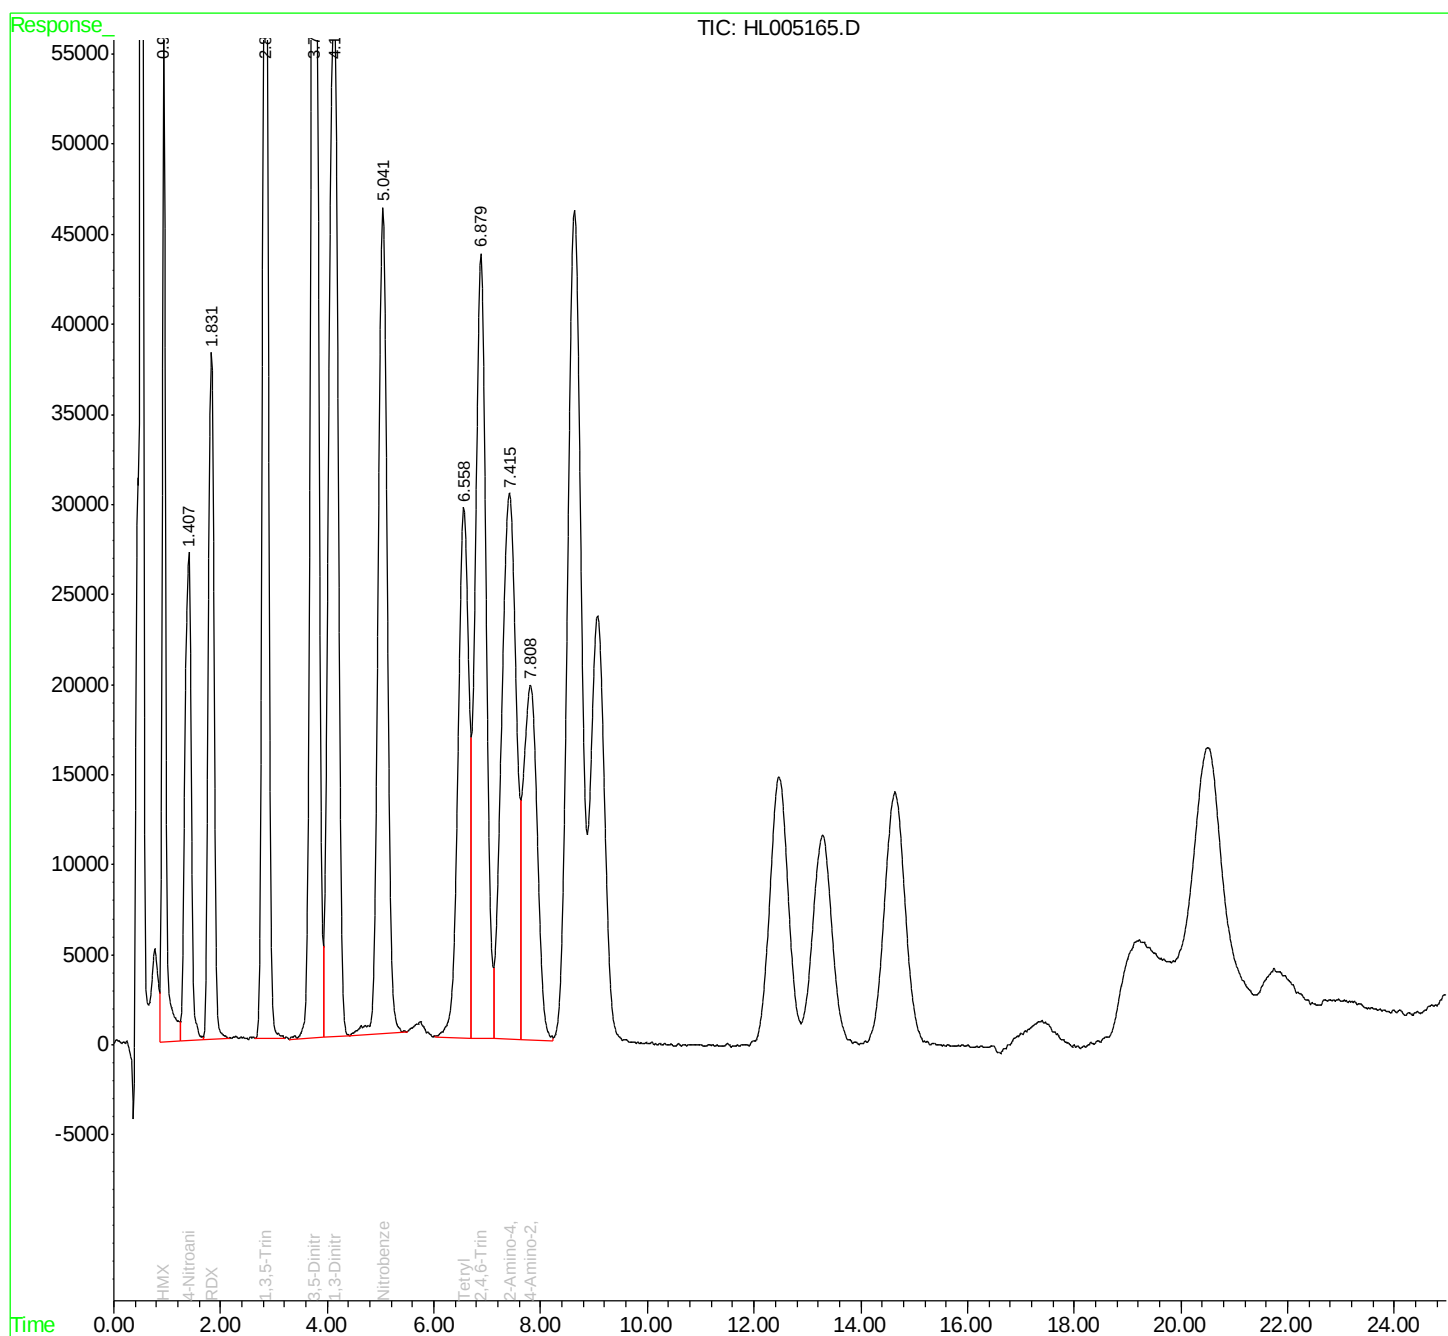


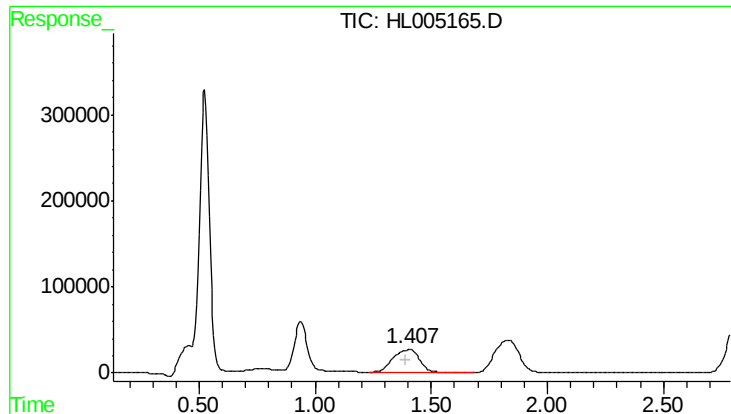

#1 4-Nitroaniline


R.T.: 1.404 min
 Delta R.T.: 0.010 min
 Response: 2202659
 Conc: 495.00 ug/L

Instrument :
 HPLC_L
 LabSampleId :
 HTSDCCC0500

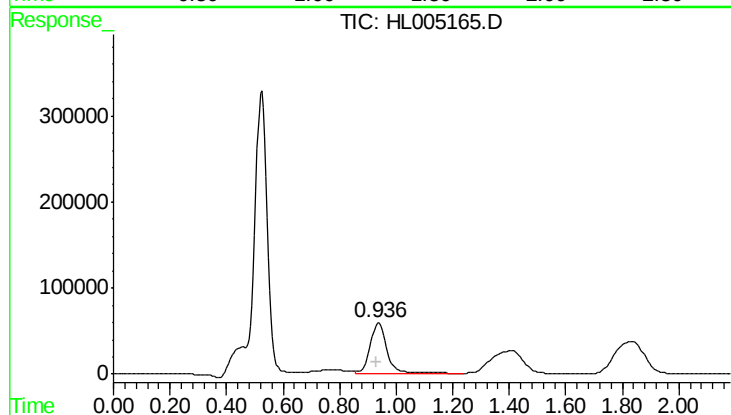


#2 HMX

R.T.: 0.938 min
 Delta R.T.: 0.010 min
 Response: 2577783
 Conc: 550.58 ug/L

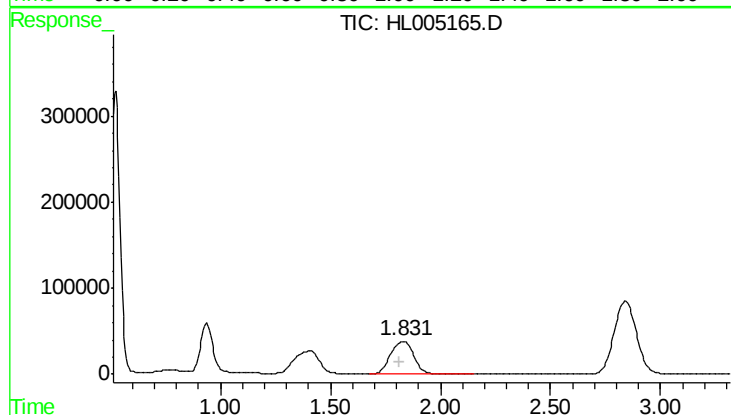


#3 RDX

R.T.: 1.831 min
 Delta R.T.: 0.014 min
 Response: 2780752
 Conc: 521.11 ug/L

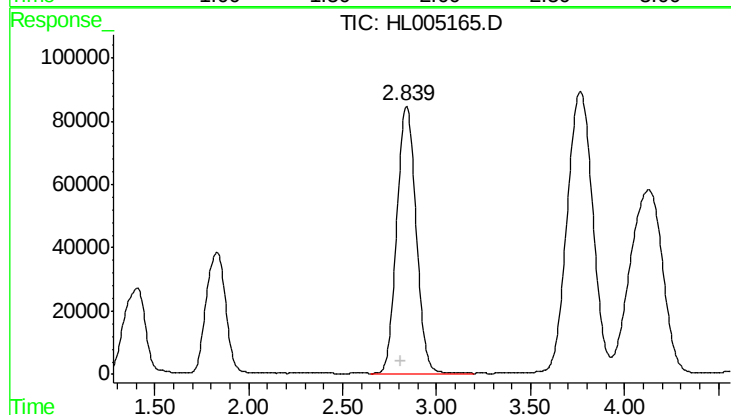

#4 1,3,5-Trinitrobenzene


R.T.: 2.841 min
 Delta R.T.: 0.032 min
 Response: 6011252
 Conc: 511.69 ug/L

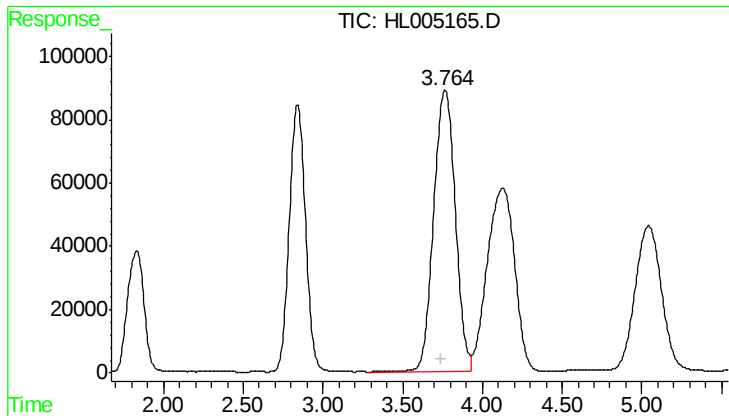

#5 3,5-Dinitroaniline


R.T.: 3.766 min
Delta R.T.: 0.024 min
Response: 8400770
Conc: 498.66 ng/ml

Instrument :
HPLC_L
LabSampleId :
HTSDCCC0500

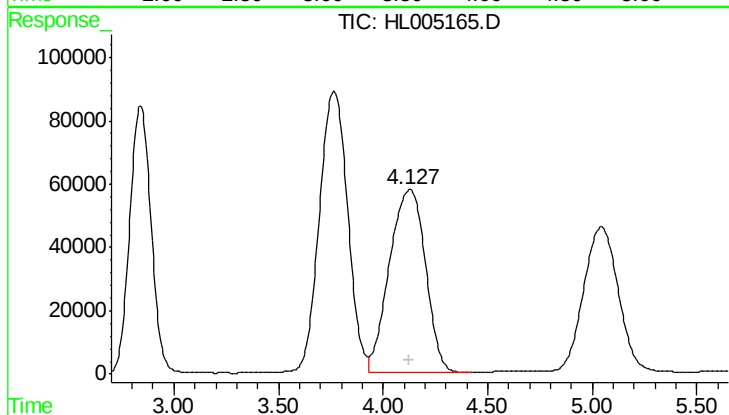


#6 1,3-Dinitrobenzene

R.T.: 4.128 min
Delta R.T.: 0.005 min
Response: 6955027
Conc: 491.48 ug/L

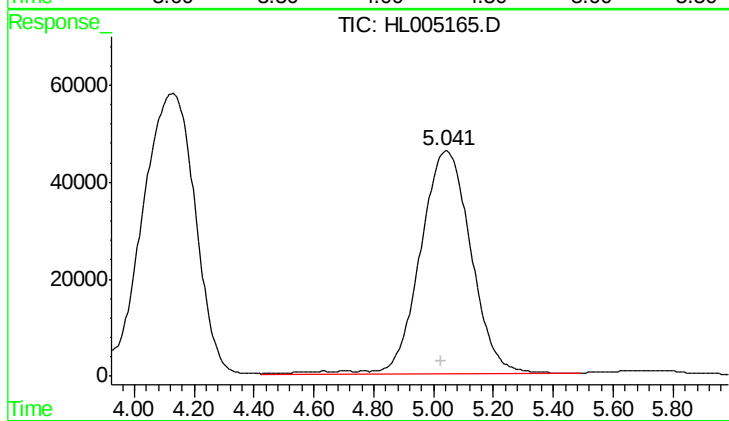


#7 Nitrobenzene

R.T.: 5.043 min
Delta R.T.: 0.018 min
Response: 5398733
Conc: 512.73 ug/L

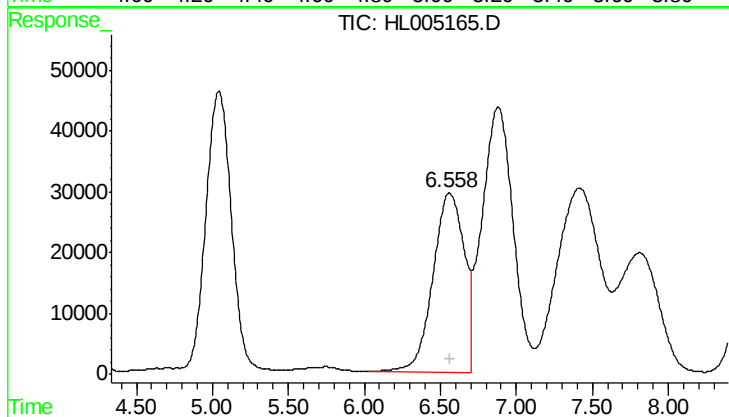

#8 Tetryl


R.T.: 6.561 min
Delta R.T.: 0.001 min
Response: 4230786
Conc: 548.00 ug/L

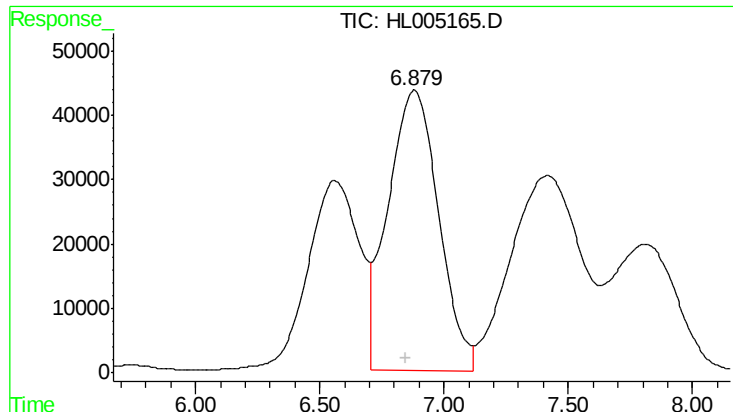

#9 2,4,6-Trinitrotoluene


R.T.: 6.880 min
Delta R.T.: 0.035 min
Response: 6200828
Conc: 514.15 ug/L

Instrument :
HPLC_L
LabSampleId :
HTSDCCC0500

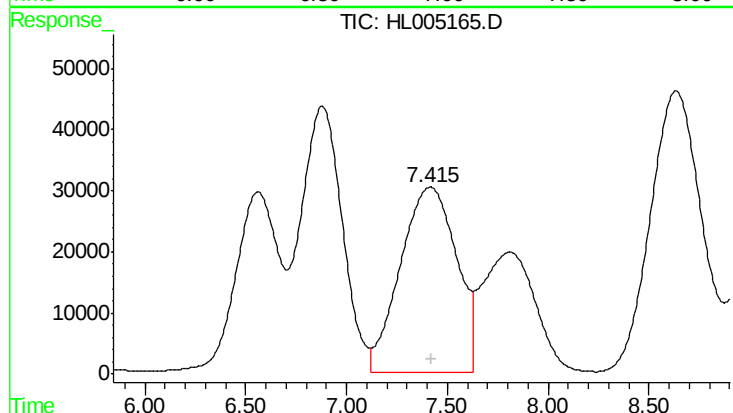

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.416 min
Delta R.T.: -0.007 min
Response: 5890644
Conc: 481.21 ug/L

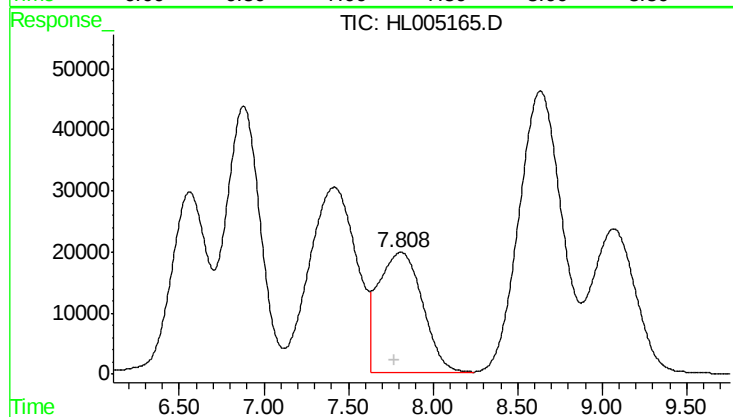

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.810 min
Delta R.T.: 0.042 min
Response: 3593096
Conc: 551.74 ug/L