

Data File : H:\VOL1\HPLC\HPLC L\120402\HL002503.D Vial: 1  
Acq On : 02-Apr-2012, 16:00 Operator: HLM  
Sample : I.BLK Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Apr 3 11:35 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Mon Apr 02 17:23:44 2012  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds


|       |      |        |       |            |
|-------|------|--------|-------|------------|
| 18) T | PETN | 19.79f | 10970 | 1.108 ug/L |
|-------|------|--------|-------|------------|


## Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120402\HL002503.D Vial: 1  
Acq On : 02-Apr-2012, 16:00 Operator: HLM  
Sample : I.BLK Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Apr 3 11:35 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Mon Apr 02 17:23:44 2012  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

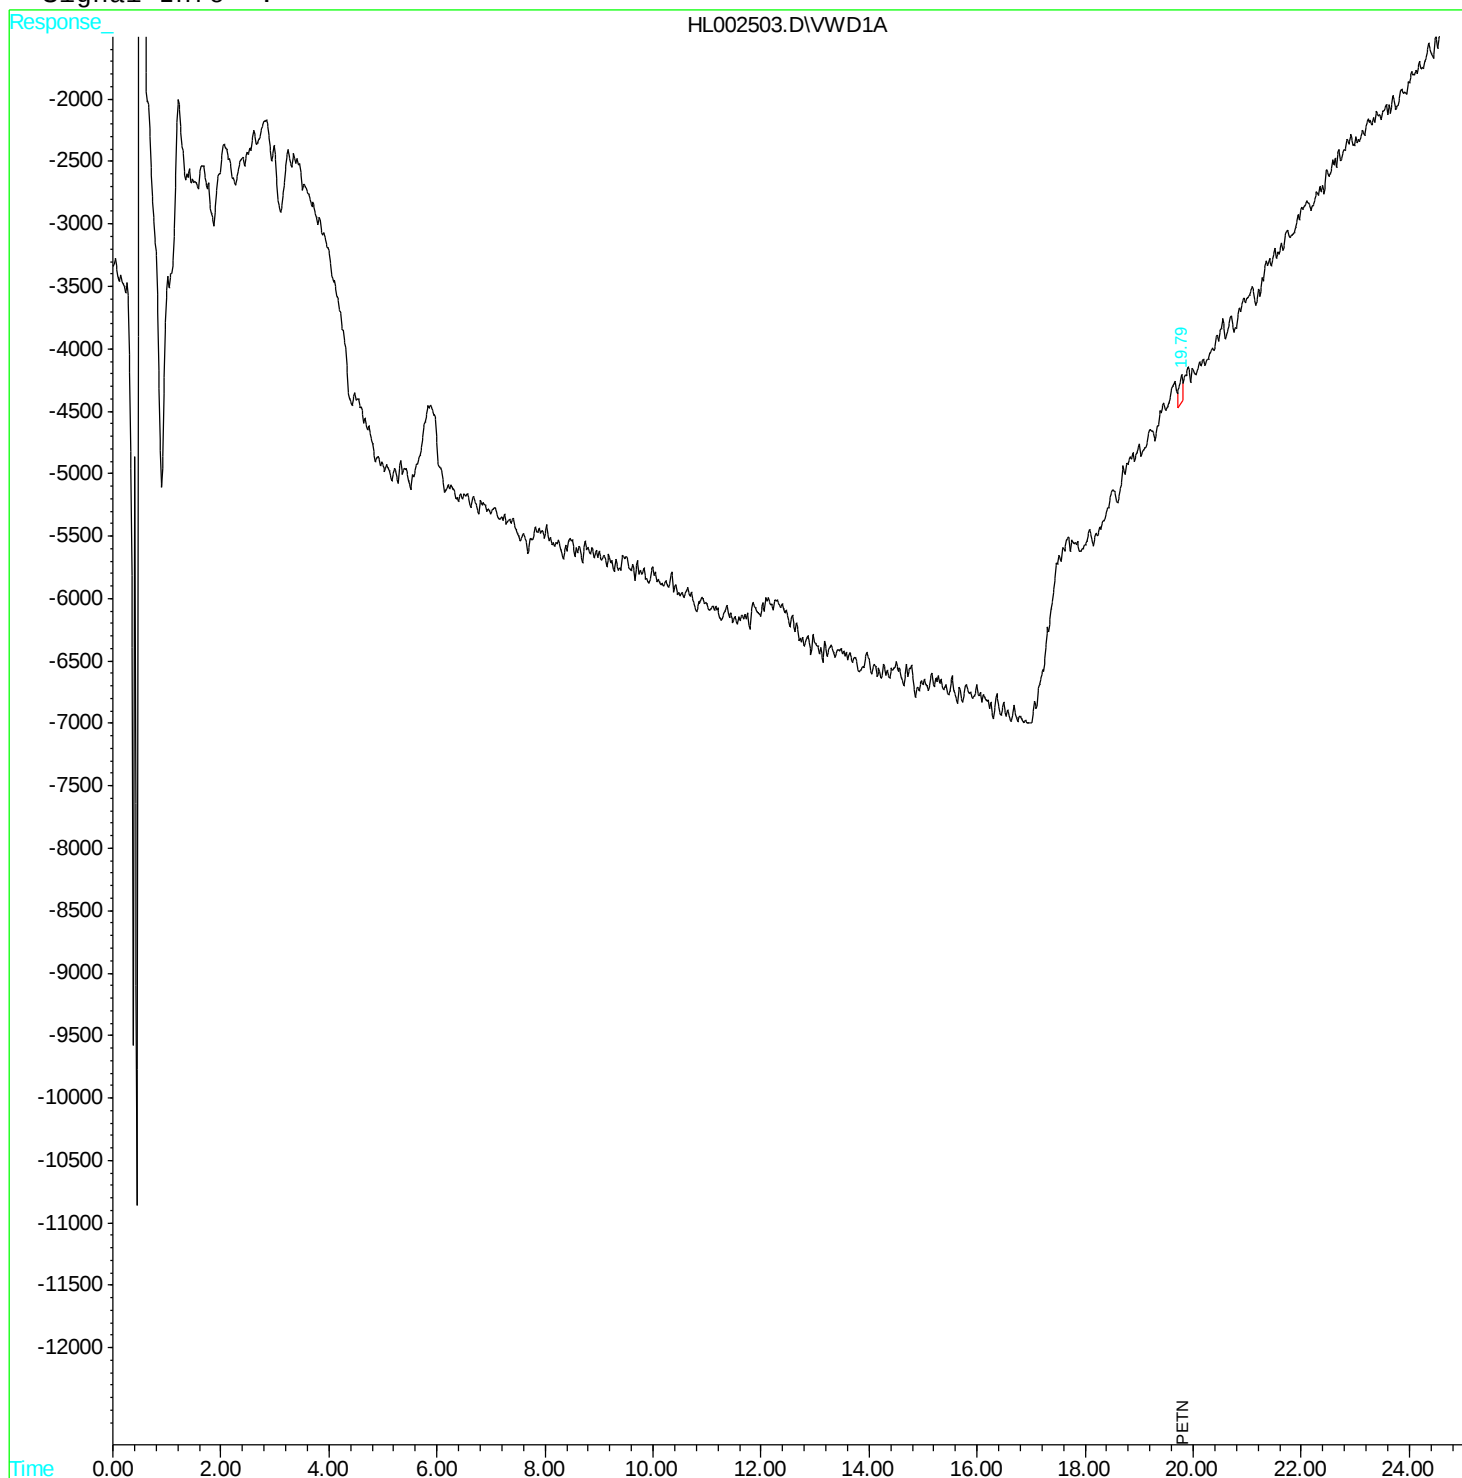

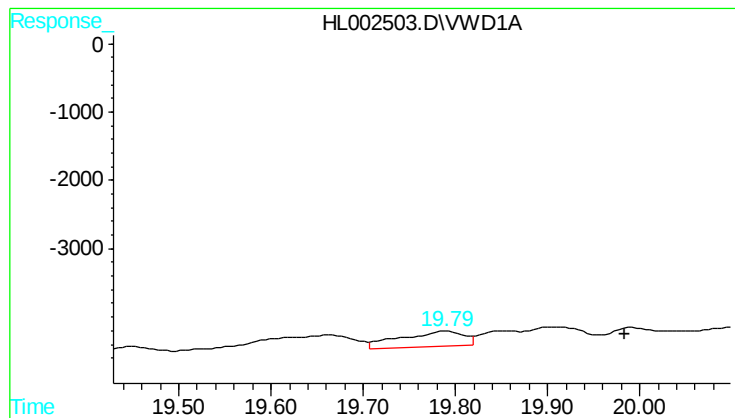

#18 PETN

R.T.: 19.789 min  
Delta R.T.: -0.195 min  
Response: 10970  
Conc: 1.11 ug/L