

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002557.D Vial: 50
Acq On : 03-Apr-2012, 16:43 Operator: HLM
Sample : D1945-01MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	644461	169.209 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 56.40%

Target Compounds


17) T	Nitroalvcerin	6.38	158508	2775.984 ug/L
18) T	PETN	19.99f	395434	39.934 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002557.D Vial: 50
 Acq On : 03-Apr-2012, 16:43 Operator: HLM
 Sample : D1945-01MSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Tue Apr 03 15:27:42 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

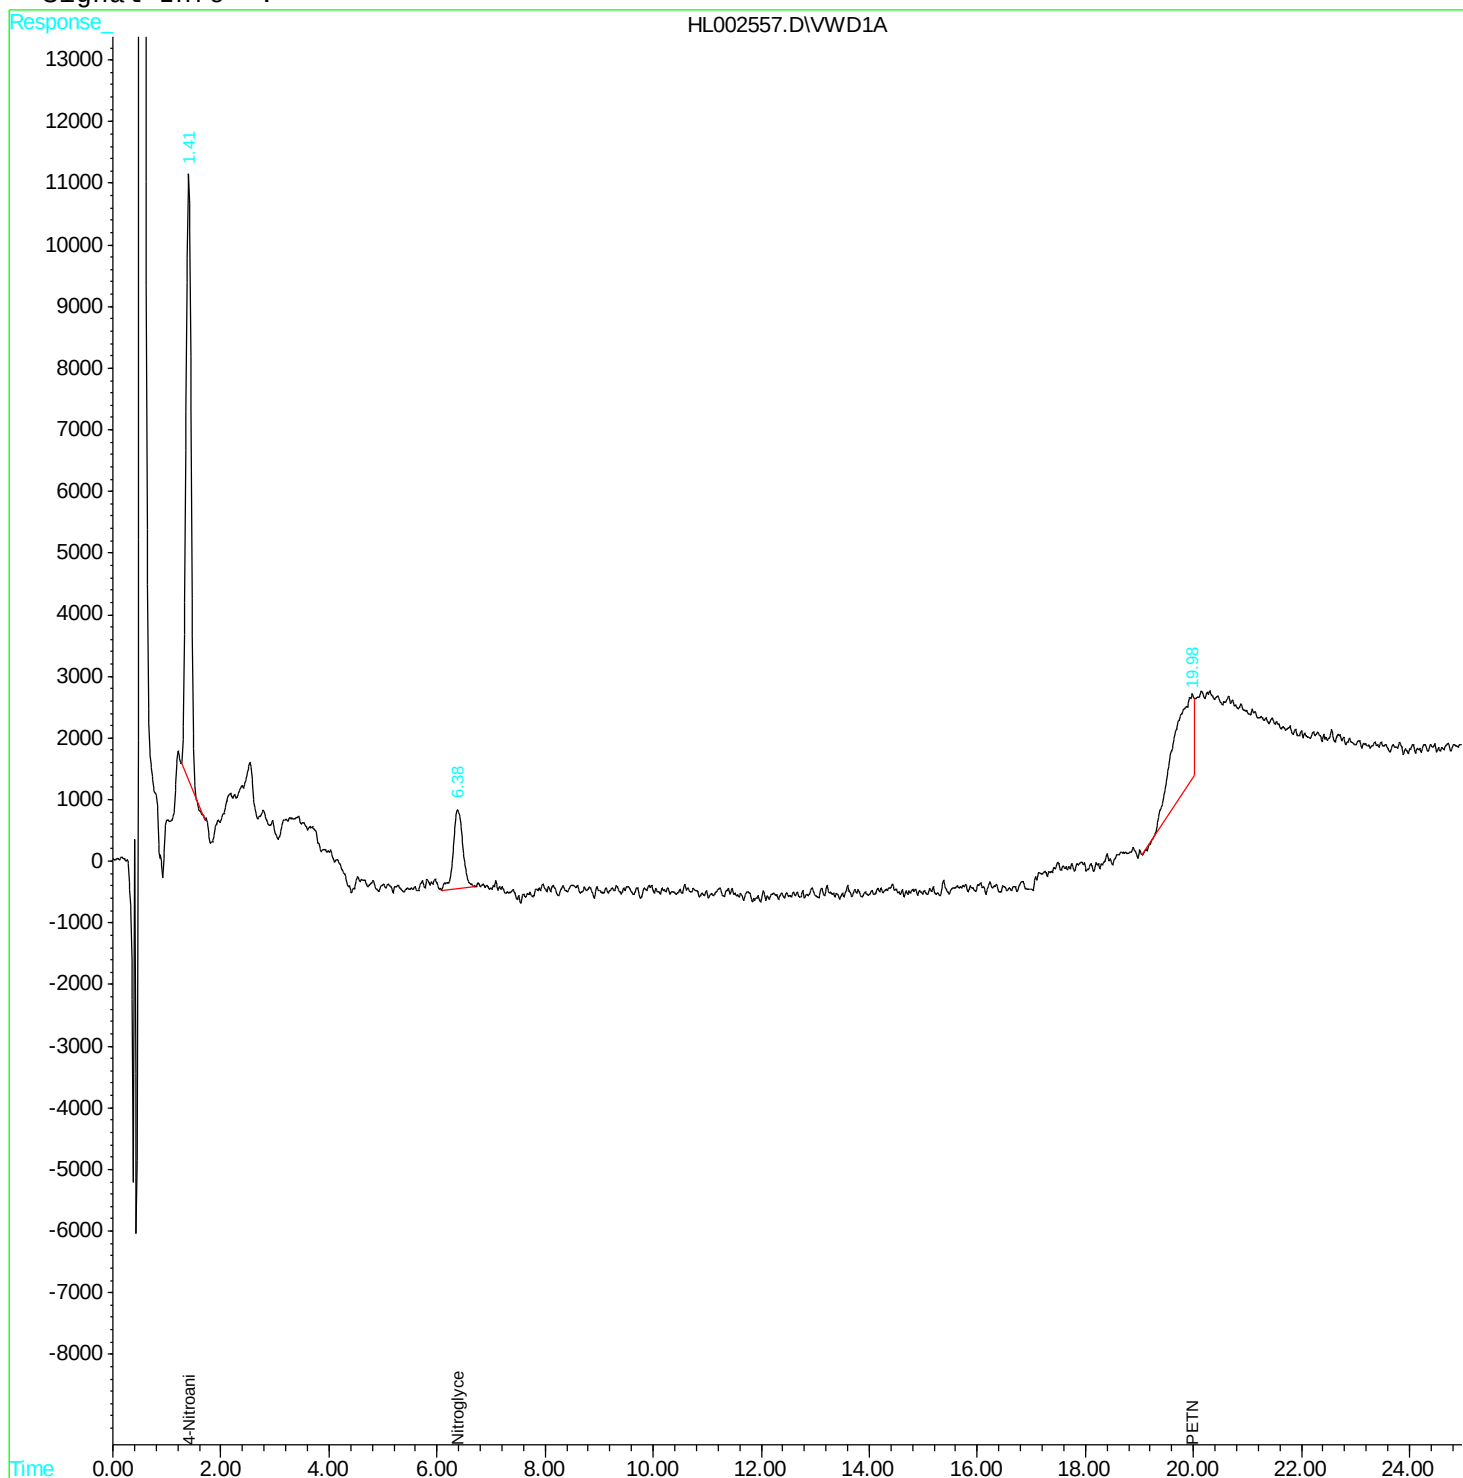

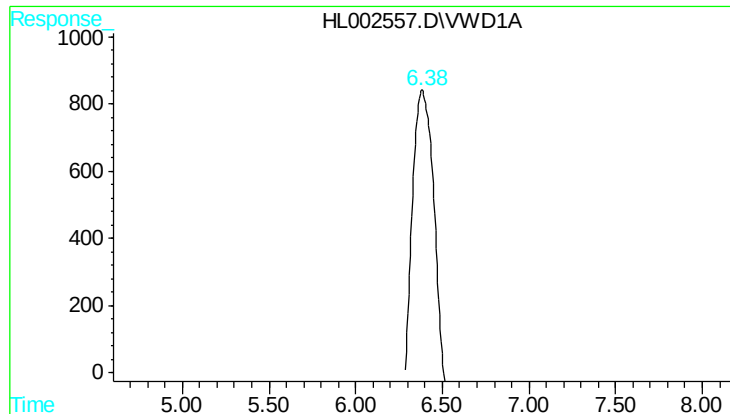

#17 Nitroglycerin

R.T.: 6.384 min
Delta R.T.: -0.005 min
Response: 158508
Conc: 2775.98 ug/L

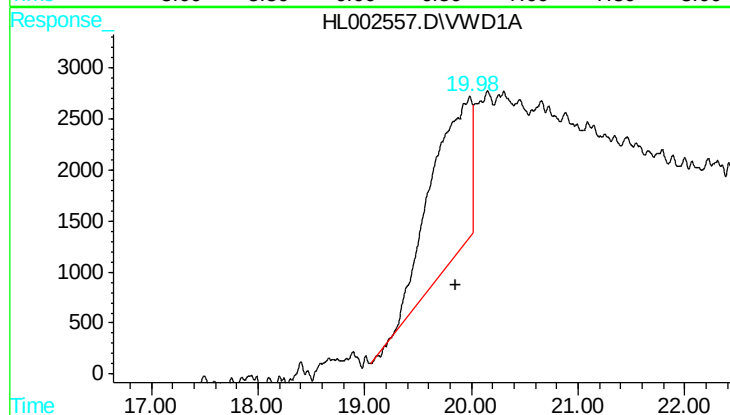

#18 PETN

R.T.: 19.986 min
Delta R.T.: 0.133 min
Response: 395434
Conc: 39.93 ug/L