

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002563.D Vial: 53
Acq On : 03-Apr-2012, 19:25 Operator: HLM
Sample : D1945-04 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	691531	181.568 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 60.52%

Target Compounds


6) T	2,4,6-Trinitrotoluene	6.92	143265	12.044 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.41	66095	5.893 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002563.D Vial: 53
Acq On : 03-Apr-2012, 19:25 Operator: HLM
Sample : D1945-04 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. :
Signal Phase :
Signal Info :

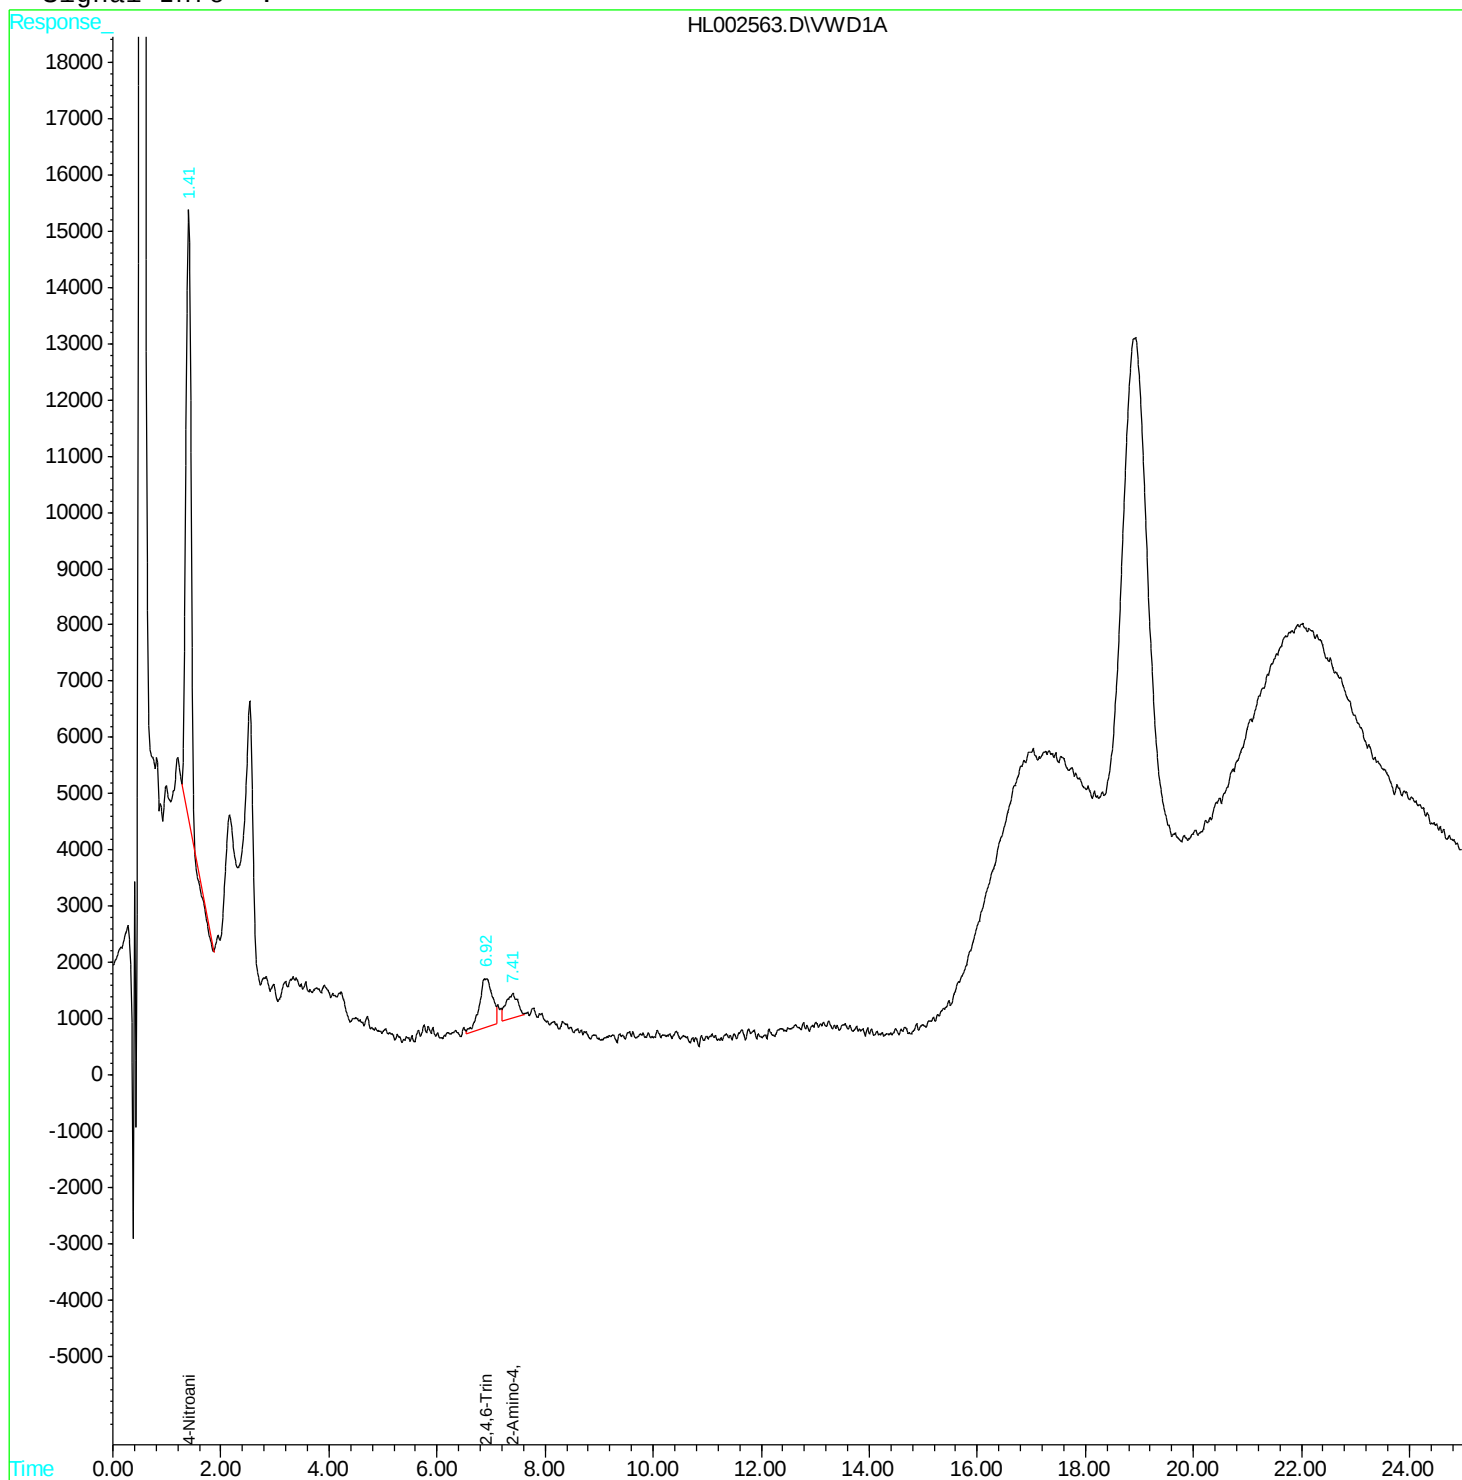

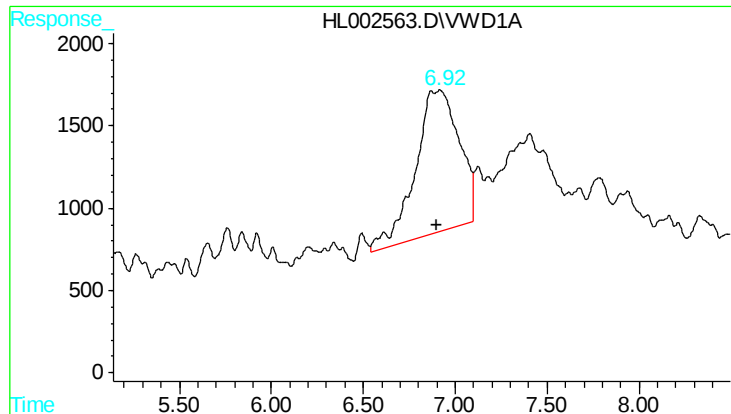

#6 2,4,6-Trinitrotoluene

R.T.: 6.917 min
Delta R.T.: 0.018 min
Response: 143265
Conc: 12.04 ug/L

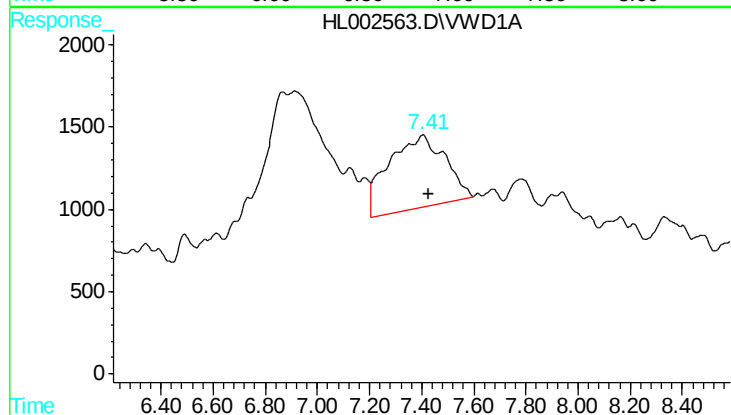

#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.406 min
Delta R.T.: -0.021 min
Response: 66095
Conc: 5.89 ug/L