

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002565.D Vial: 55
Acq On : 03-Apr-2012, 20:19 Operator: HLM
Sample : D1945-06 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	650204	170.718 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 56.91%

Target Compounds


7) T	2-Amino-4,6-dinitrotoluene	7.38f	1940	0.173 ug/L
------	----------------------------	-------	------	------------


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002565.D Vial: 55
Acq On : 03-Apr-2012, 20:19 Operator: HLM
Sample : D1945-06 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

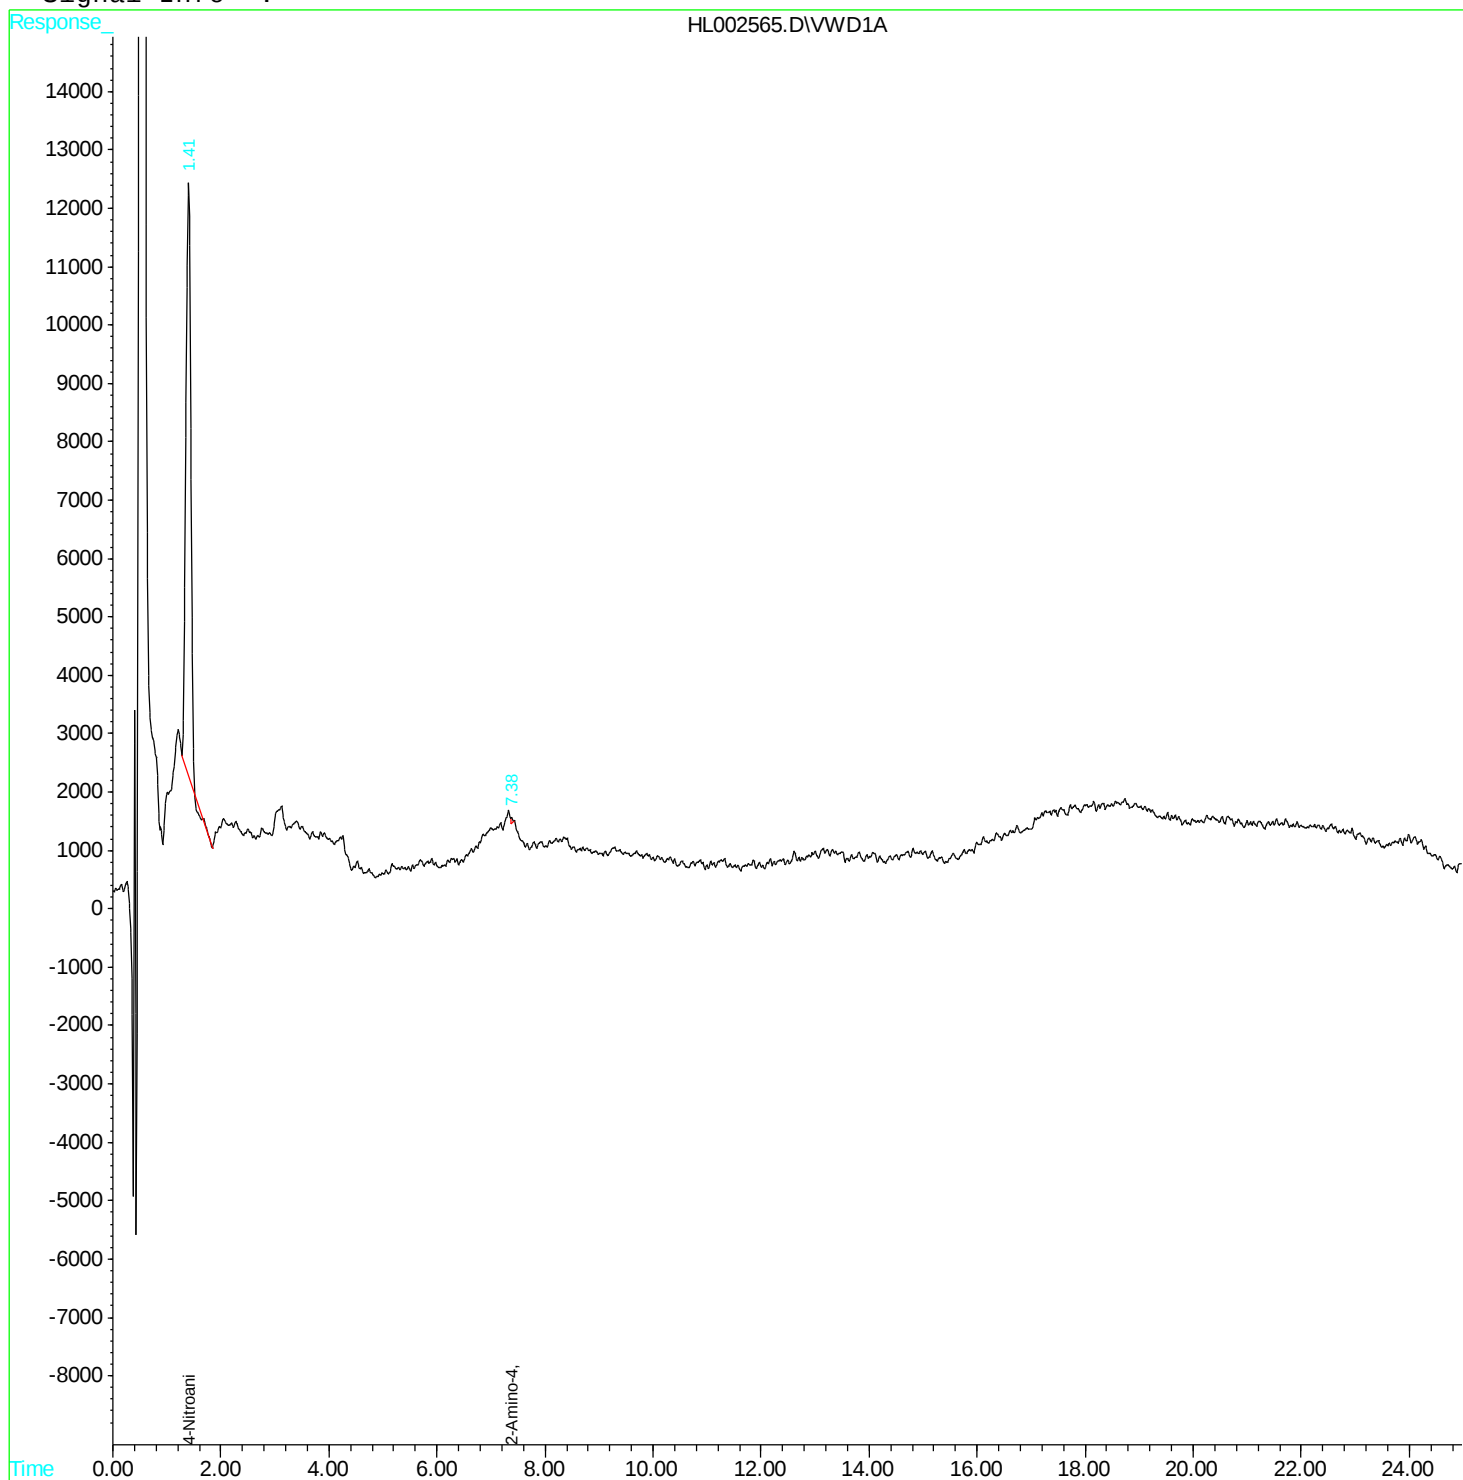

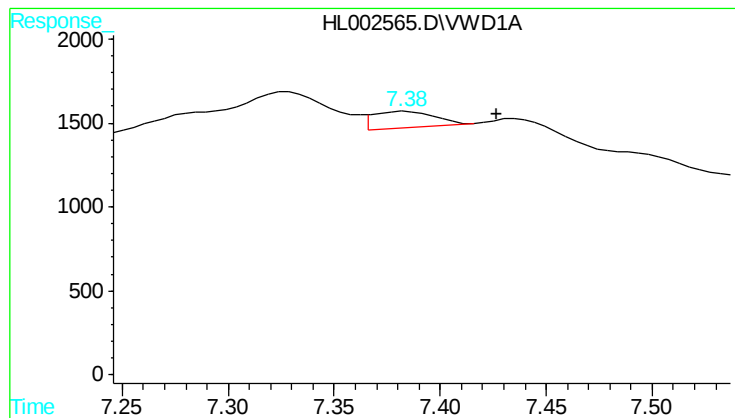

#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.384 min
Delta R.T.: -0.043 min
Response: 1940
Conc: 0.17 ug/L