

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002566.D Vial: 56
Acq On : 03-Apr-2012, 20:46 Operator: HLM
Sample : D1945-07 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	609371	159.996 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 53.33%


Target Compounds


16) T	3,5-Dinitroaniline	4.13	56038	3.336 ug/L
-------	--------------------	------	-------	------------

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002566.D Vial: 56
Acq On : 03-Apr-2012, 20:46 Operator: HLM
Sample : D1945-07 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 10:28 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

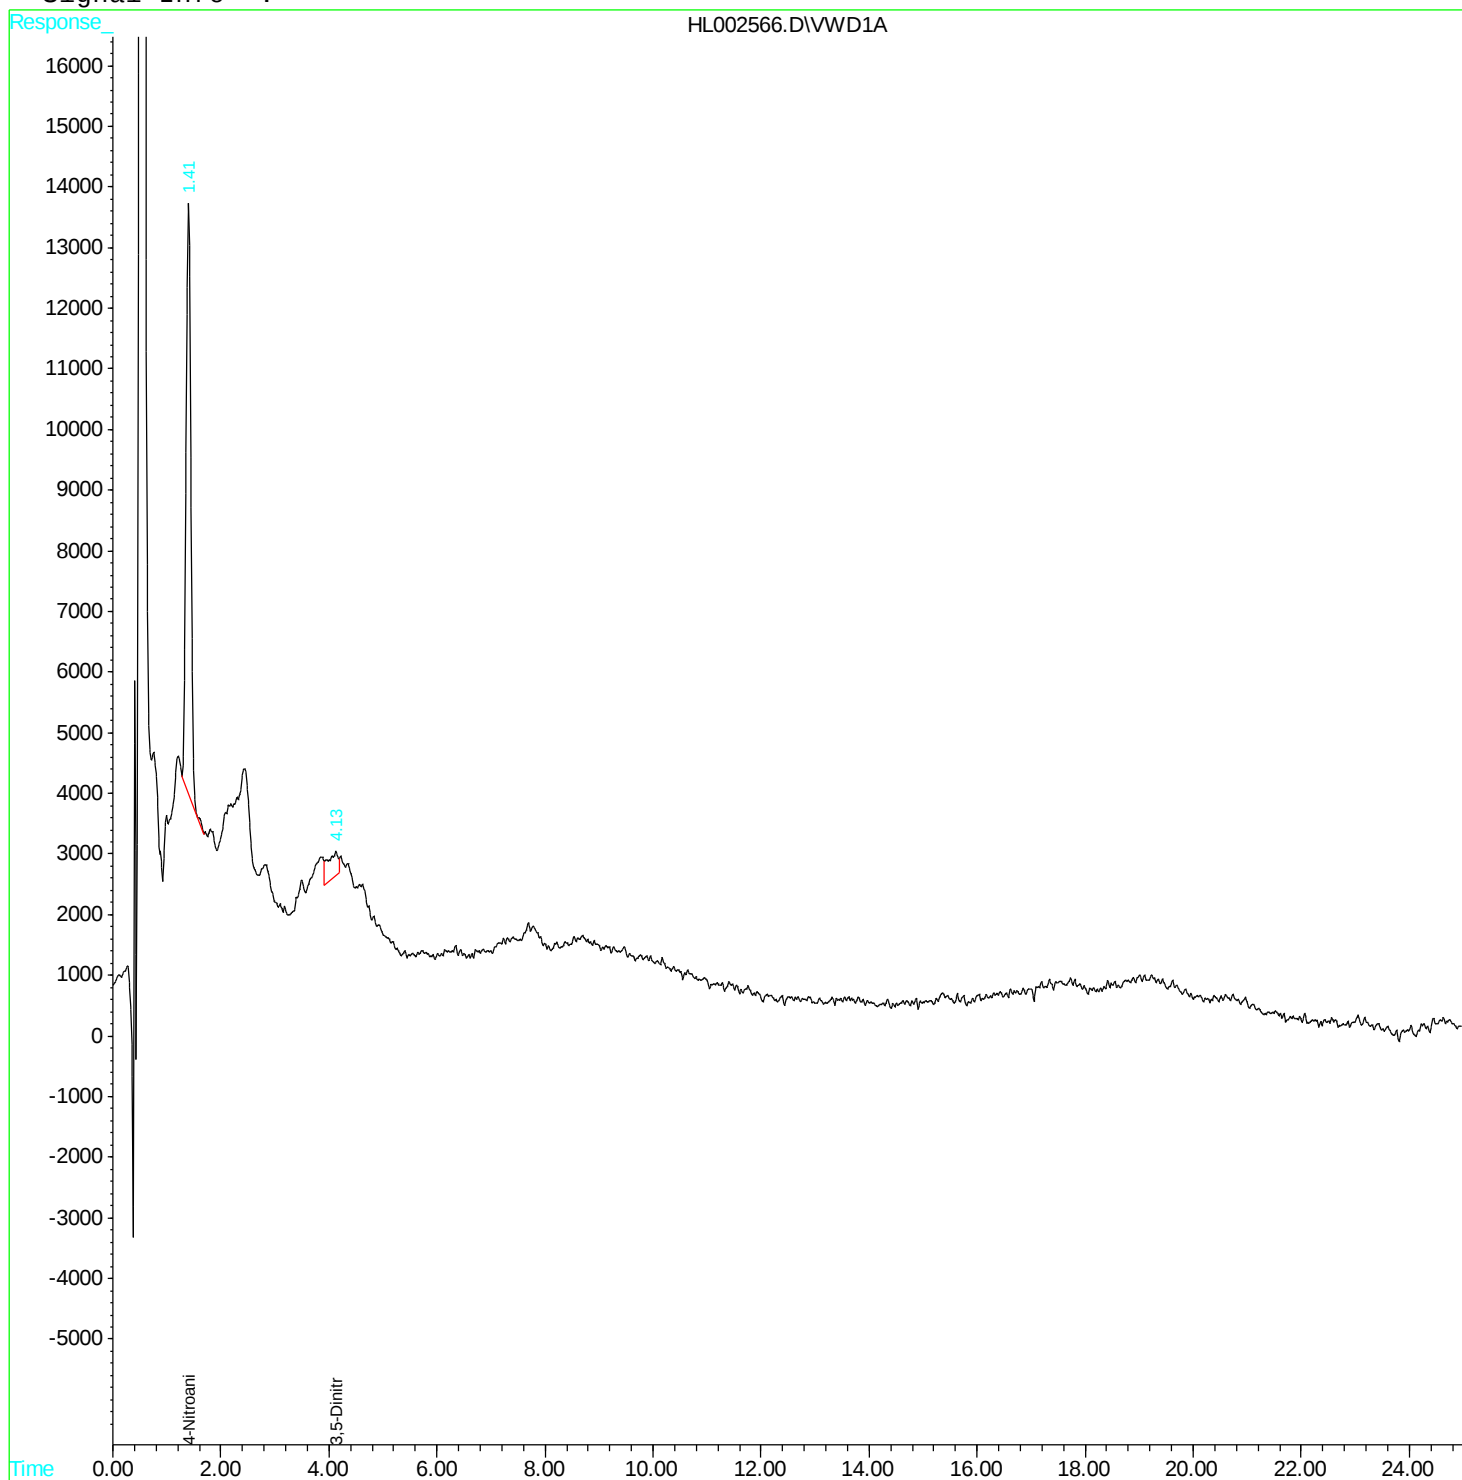

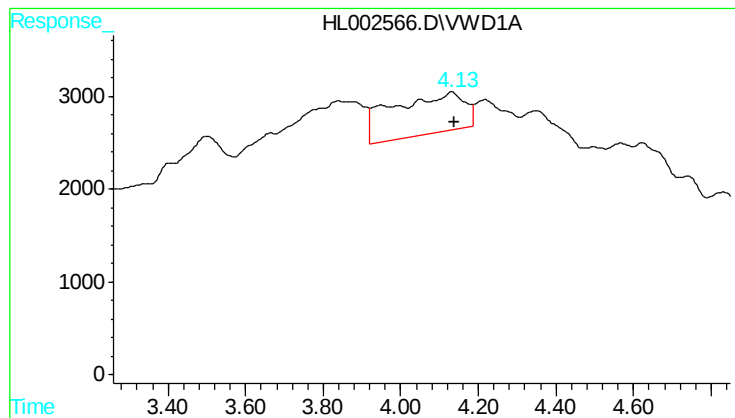

#16 3,5-Dinitroaniline

R.T.: 4.133 min
Delta R.T.: -0.006 min
Response: 56038
Conc: 3.34 ug/L