

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002595.D Vial: 79
Acq On : 04-Apr-2012, 09:49 Operator: HLM
Sample : D1953-02MS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 15:21 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40	669906	175.890 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 58.63%

Target Compounds


17) T	Nitroalvcerin	6.37	174311	3052.747 ug/L
18) T	PETN	20.03f	14052	1.419 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002595.D Vial: 79
Acq On : 04-Apr-2012, 09:49 Operator: HLM
Sample : D1953-02MS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 4 15:21 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Apr 03 15:27:42 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. :
Signal Phase :
Signal Info :

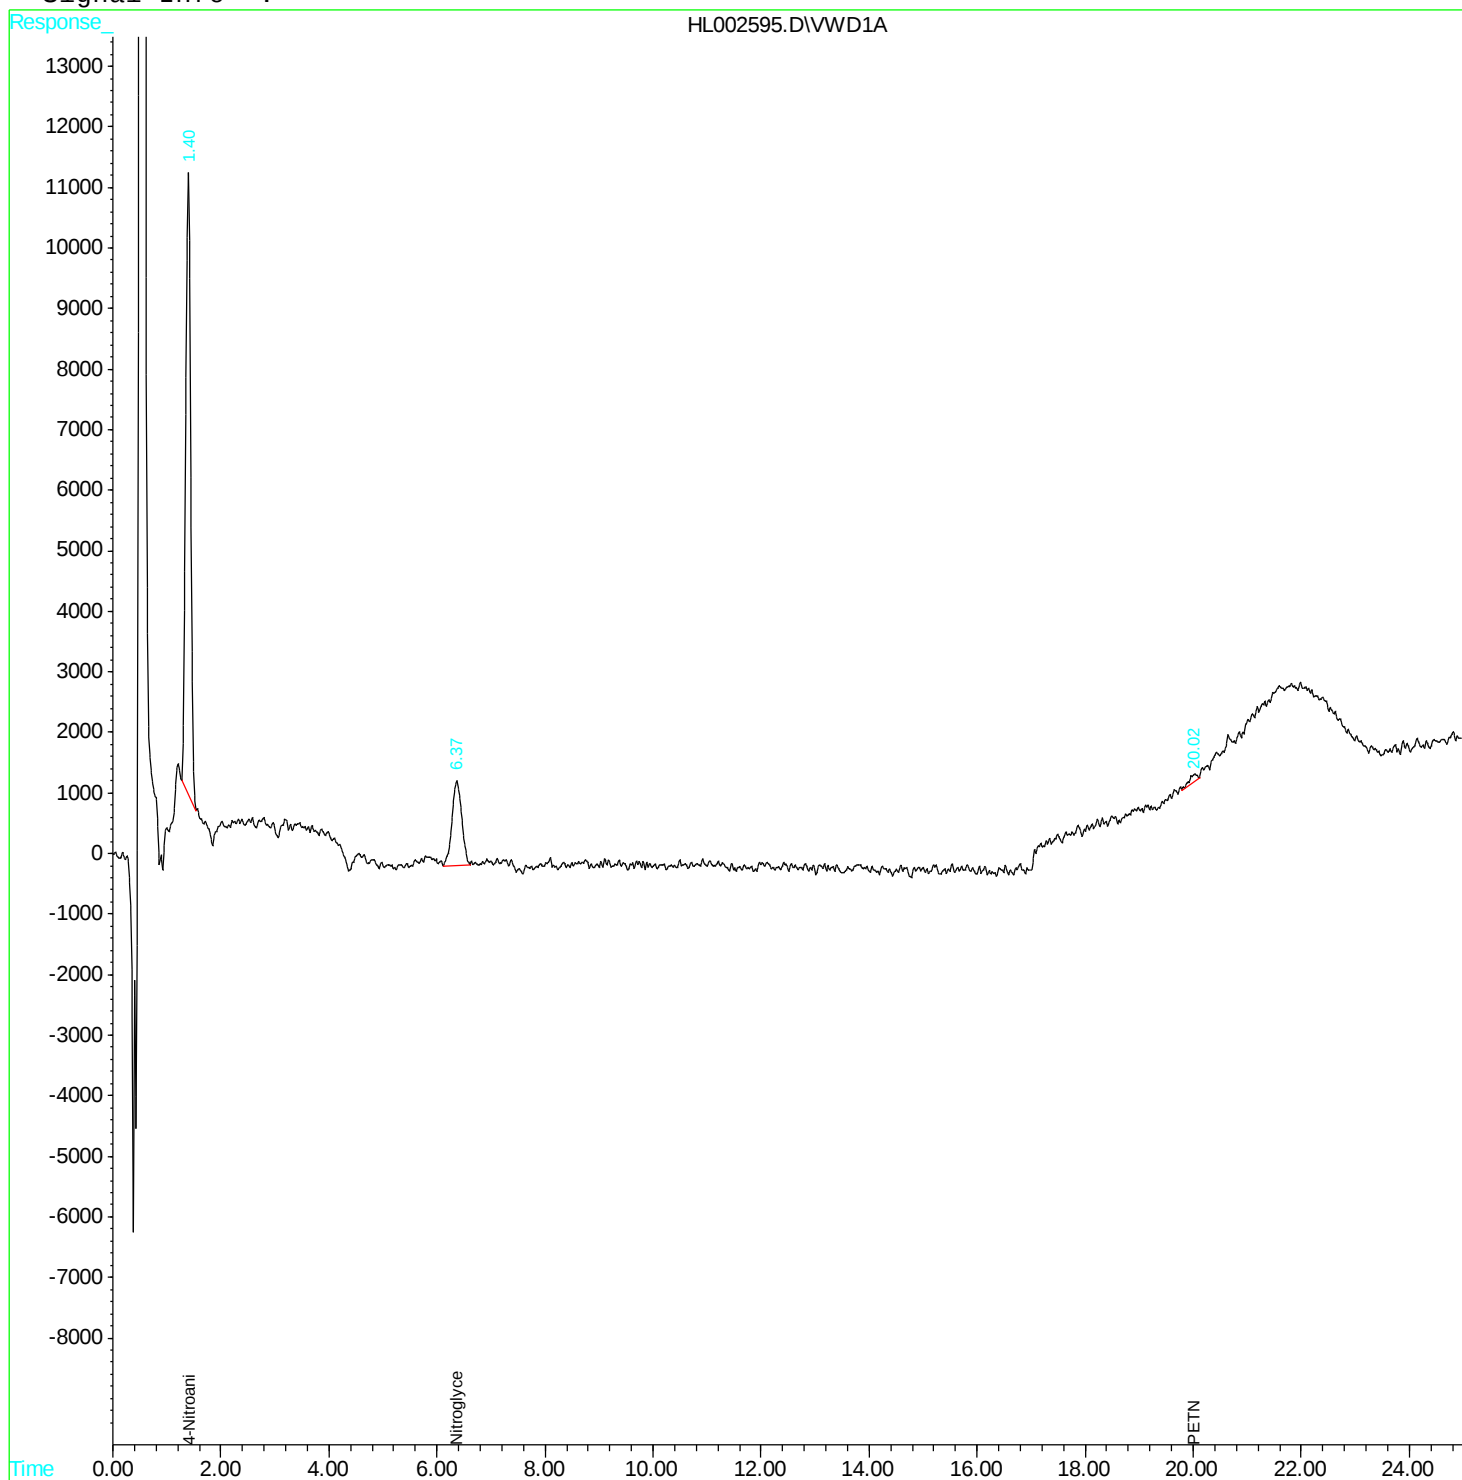

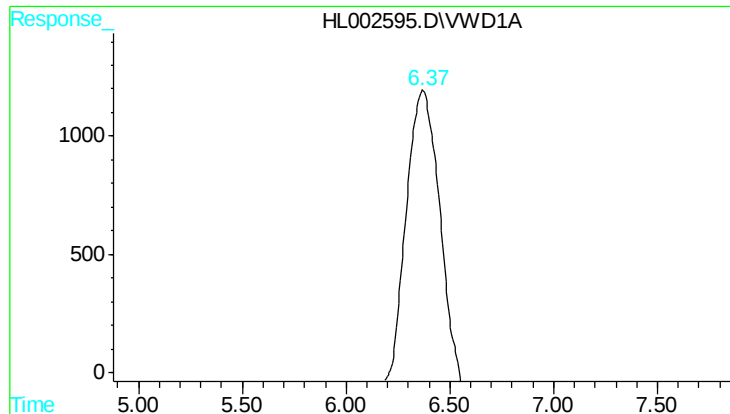

#17 Nitroglycerin

R.T.: 6.371 min
Delta R.T.: -0.017 min
Response: 174311
Conc: 3052.75 ug/L

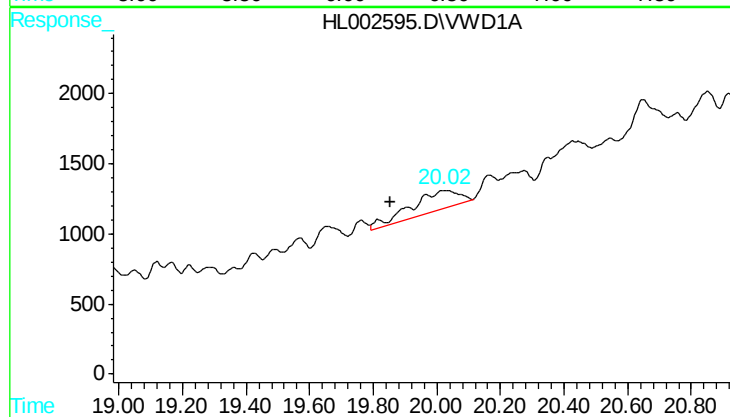

#18 PETN

R.T.: 20.028 min
Delta R.T.: 0.175 min
Response: 14052
Conc: 1.42 ug/L