

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002606.D Vial: 87
 Acq On : 04-Apr-2012, 14:46 Operator: HLM
 Sample : D1953-09MS1 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 4 15:22 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Tue Apr 03 15:27:42 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	457204	120.043 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 40.01%

Target Compounds


2) T	HMX	0.94	541242	123.447 ug/L
3) T	RDX	1.81	561209	102.883 ug/L
4) T	1,3,5-Trinitrobenzene	2.83	1359168	106.773 ug/L
5) T	Tetryl	6.55	818189	90.411 ug/L
6) T	2,4,6-Trinitrotoluene	6.89	1328140	111.652 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.41	1268296	113.081 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.77	827303	107.242 ug/L
9) T	2,4-Dinitrotoluene	8.62	1773061	104.469 ug/L
10) T	2,6-Dinitrotoluene	9.03	943240	106.401 ug/L
11) T	1,3-Dinitrobenzene	3.76	1996726	111.151 ug/L
12) T	Nitrobenzene	5.07	1242083	117.871 ug/L
13) T	2-Nitrotoluene	12.46	772135	110.866 ug/L
14) T	3-Nitrotoluene	14.60	816616	114.218 ug/L
15) T	4-Nitrotoluene	13.27	676274	117.376 ug/L
16) T	3,5-Dinitroaniline	4.12	1503439	89.512 ug/L
18) T	PETN	19.77	834503	84.275 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120403\HL002606.D Vial: 87
 Acq On : 04-Apr-2012, 14:46 Operator: HLM
 Sample : D1953-09MS1 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 4 15:22 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Tue Apr 03 15:27:42 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

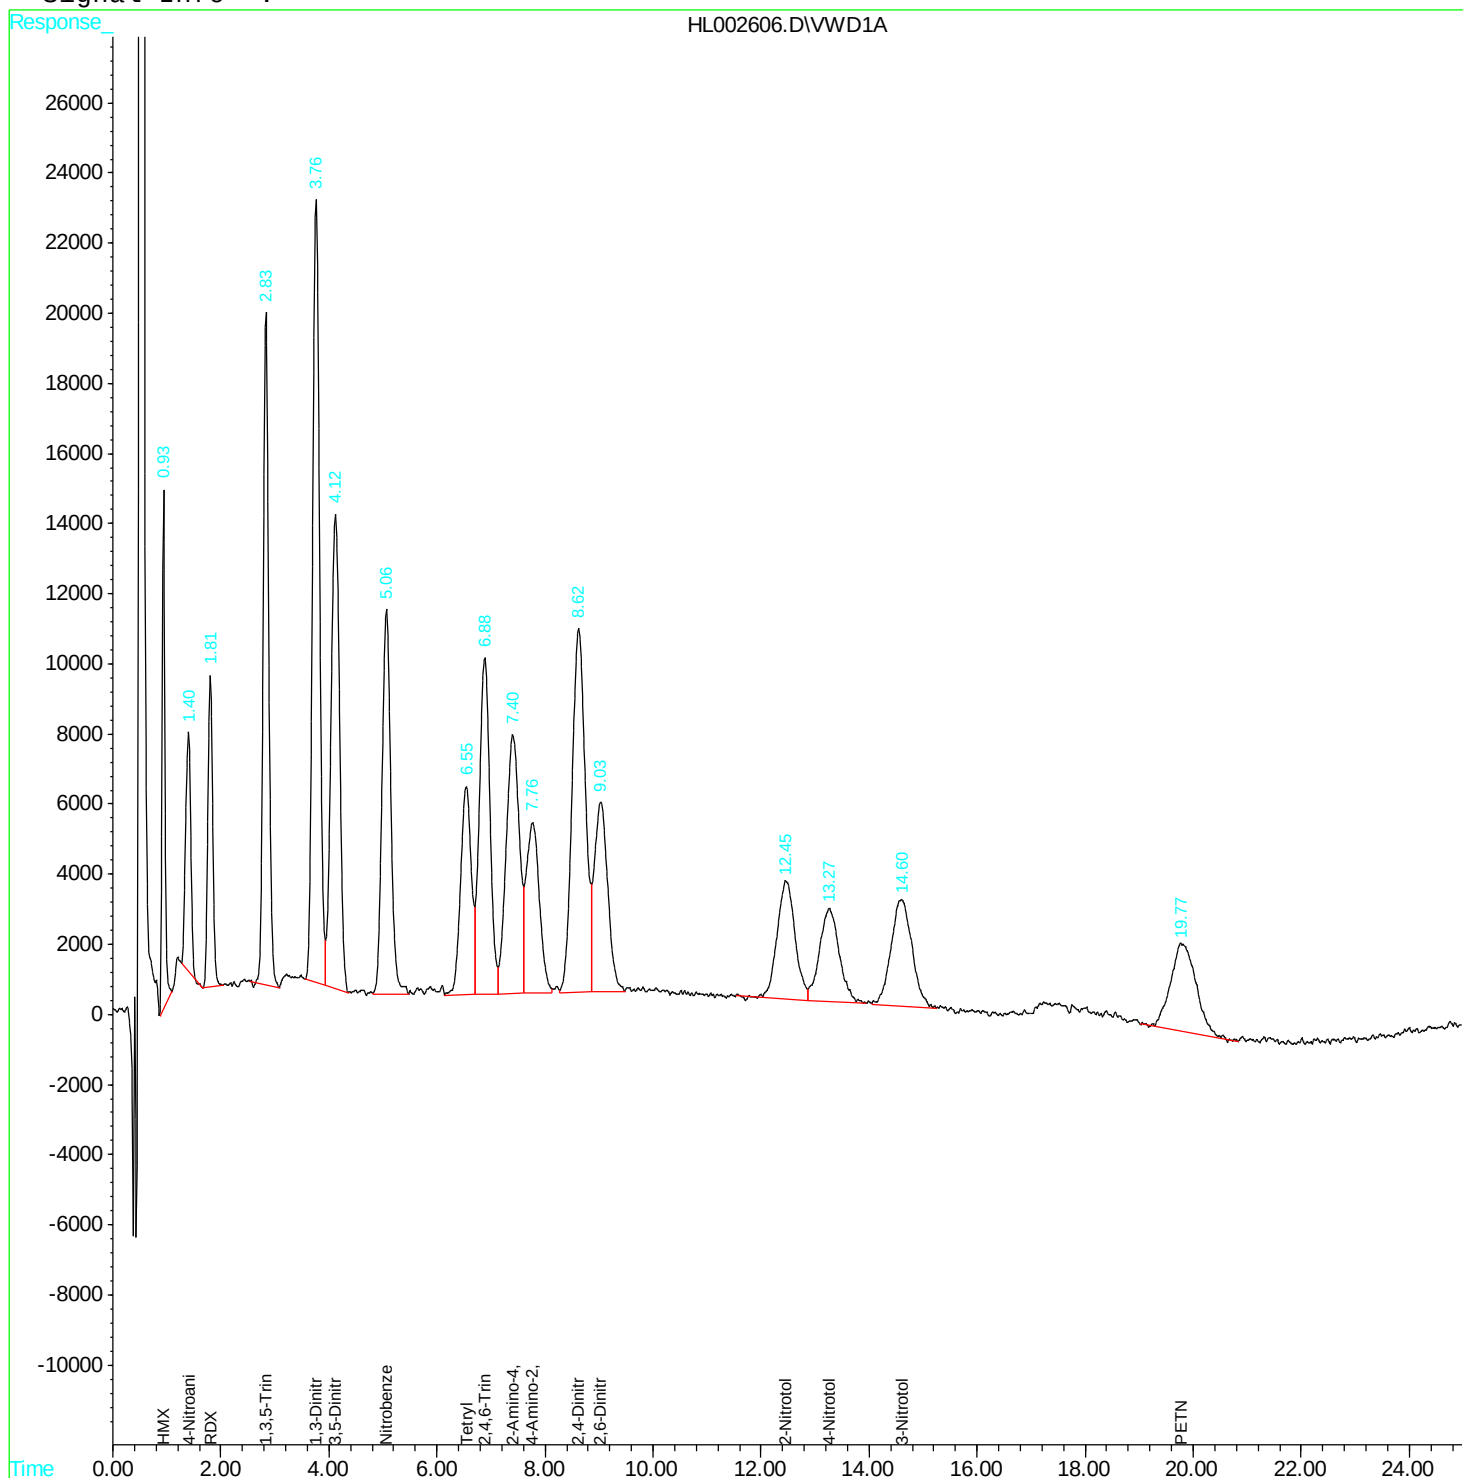

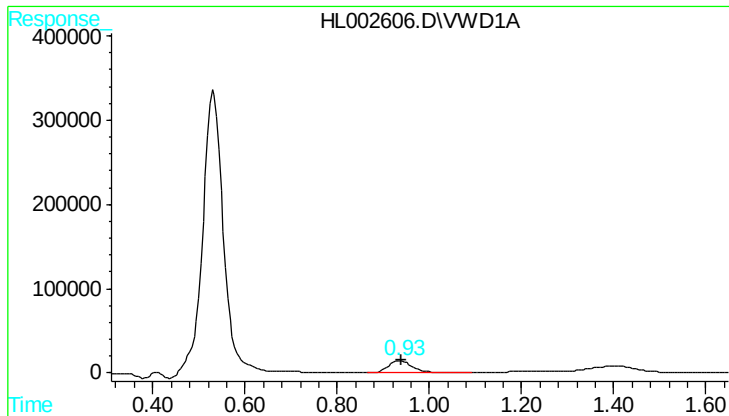


#2 HMX

R.T.: 0.937 min
Delta R.T.: -0.002 min
Response: 541242
Conc: 123.45 ug/L

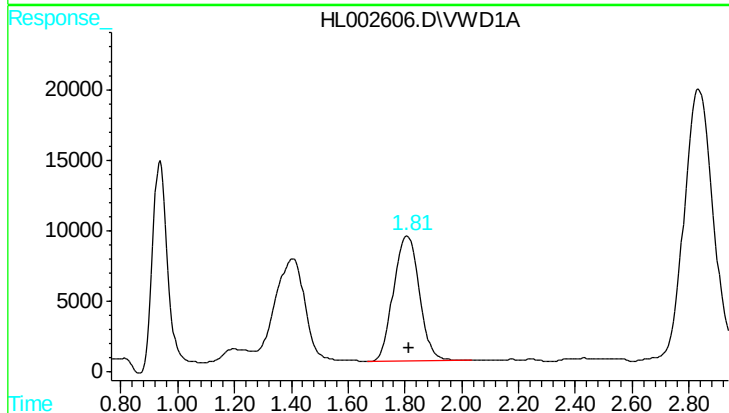


#3 RDX

R.T.: 1.808 min
Delta R.T.: -0.007 min
Response: 561209
Conc: 102.88 ug/L

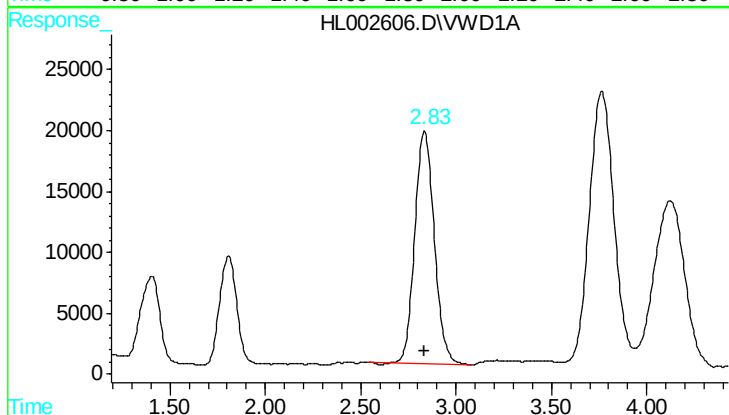


#4 1,3,5-Trinitrobenzene

R.T.: 2.835 min
Delta R.T.: 0.000 min
Response: 1359168
Conc: 106.77 ug/L

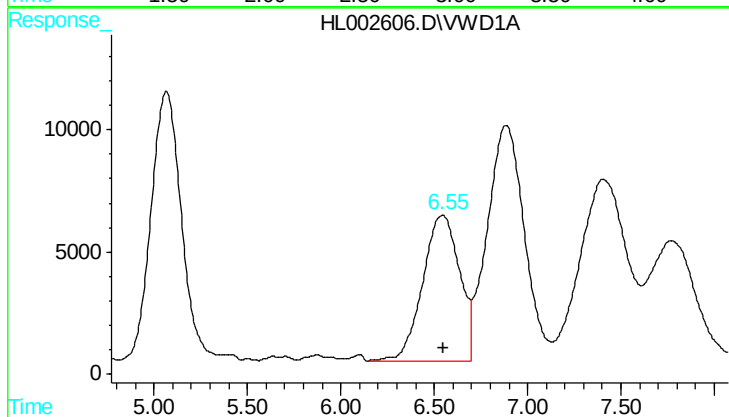


#5 Tetryl

R.T.: 6.546 min
Delta R.T.: -0.005 min
Response: 818189
Conc: 90.41 ug/L

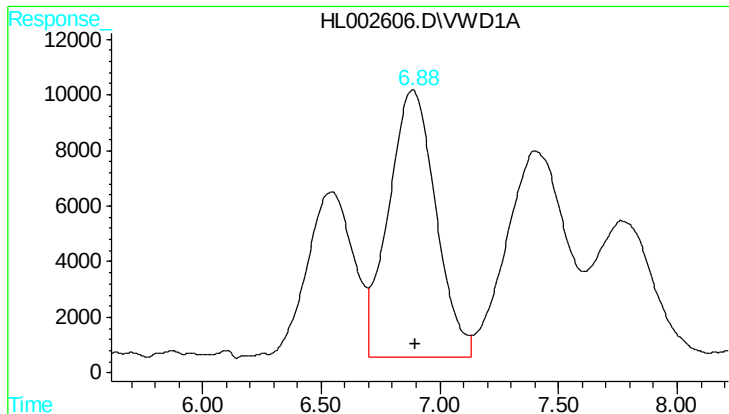


#6 2,4,6-Trinitrotoluene

R.T.: 6.887 min
Delta R.T.: -0.012 min
Response: 1328140
Conc: 111.65 ug/L

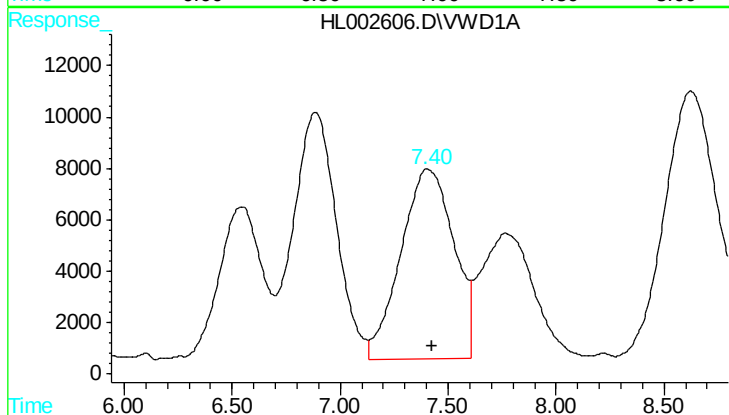


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.406 min
Delta R.T.: -0.021 min
Response: 1268296
Conc: 113.08 ug/L

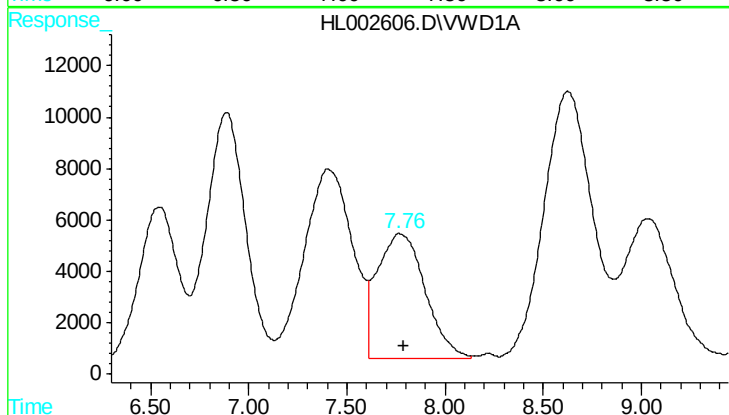


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.770 min
Delta R.T.: -0.023 min
Response: 827303
Conc: 107.24 ug/L

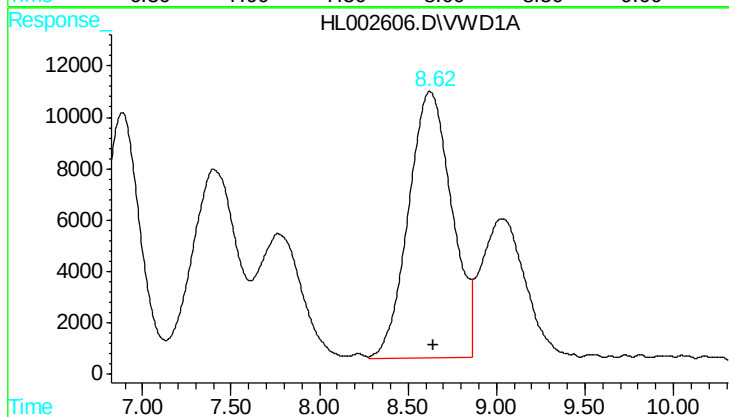


#9 2,4-Dinitrotoluene

R.T.: 8.625 min
Delta R.T.: -0.021 min
Response: 1773061
Conc: 104.47 ug/L

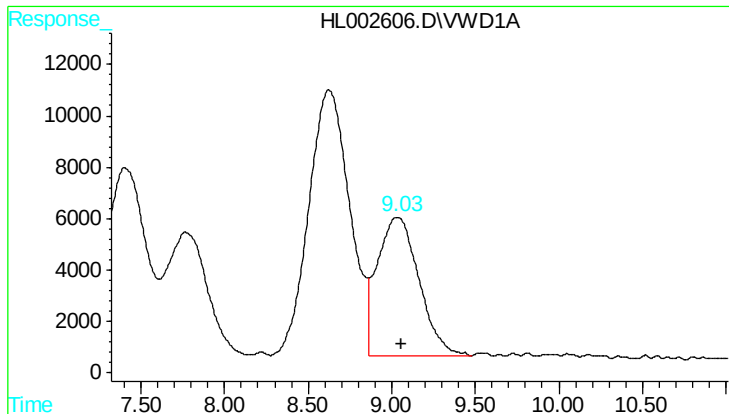


#10 2,6-Dinitrotoluene

R.T.: 9.033 min
Delta R.T.: -0.026 min
Response: 943240
Conc: 106.40 ug/L

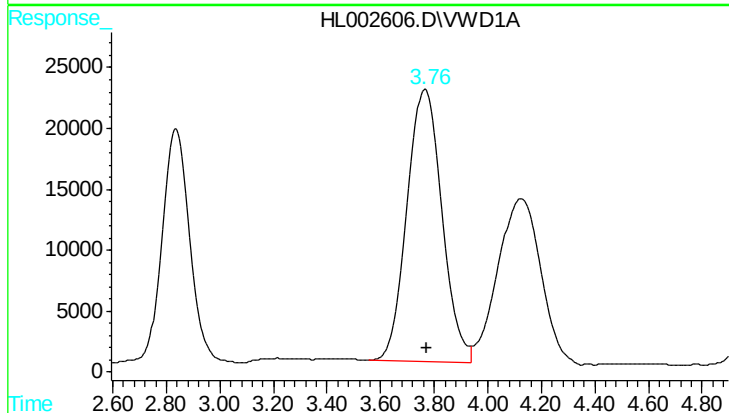


#11 1,3-Dinitrobenzene

R.T.: 3.764 min
Delta R.T.: -0.011 min
Response: 1996726
Conc: 111.15 ug/L

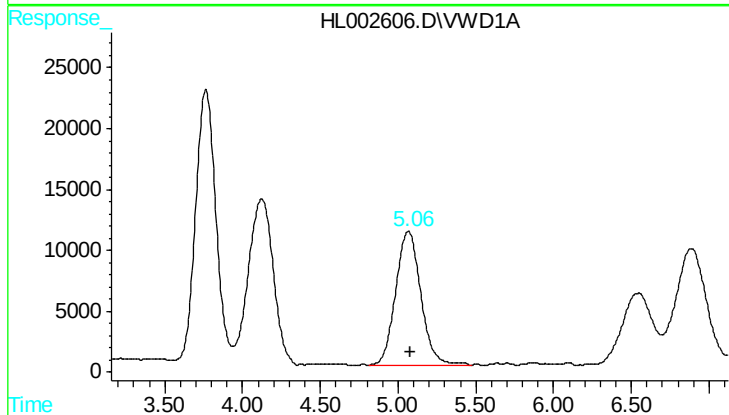


#12 Nitrobenzene

R.T.: 5.067 min
Delta R.T.: -0.016 min
Response: 1242083
Conc: 117.87 ug/L

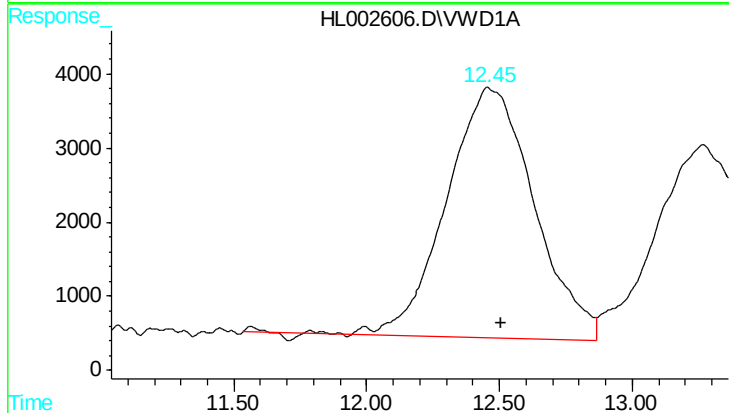


#13 2-Nitrotoluene

R.T.: 12.460 min
Delta R.T.: -0.046 min
Response: 772135
Conc: 110.87 ug/L

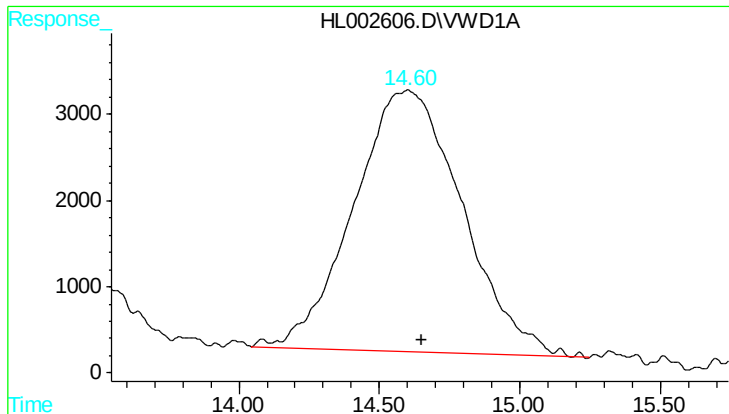


#14 3-Nitrotoluene

R.T.: 14.601 min
Delta R.T.: -0.052 min
Response: 816616
Conc: 114.22 ug/L

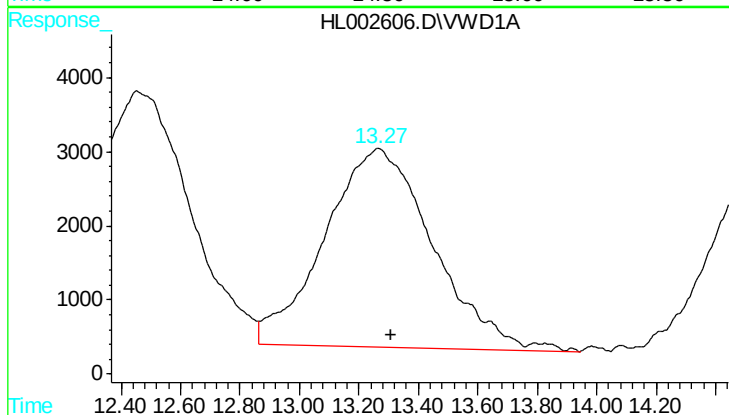


#15 4-Nitrotoluene

R.T.: 13.265 min
Delta R.T.: -0.043 min
Response: 676274
Conc: 117.38 ug/L

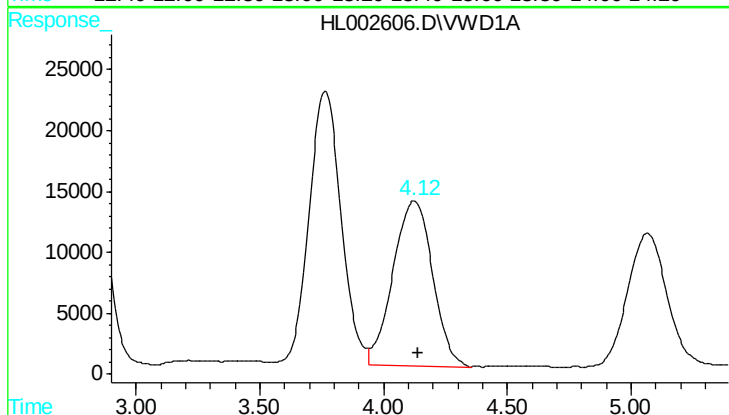

#16 3,5-Dinitroaniline

R.T.: 4.124 min
Delta R.T.: -0.014 min
Response: 1503439
Conc: 89.51 ug/L

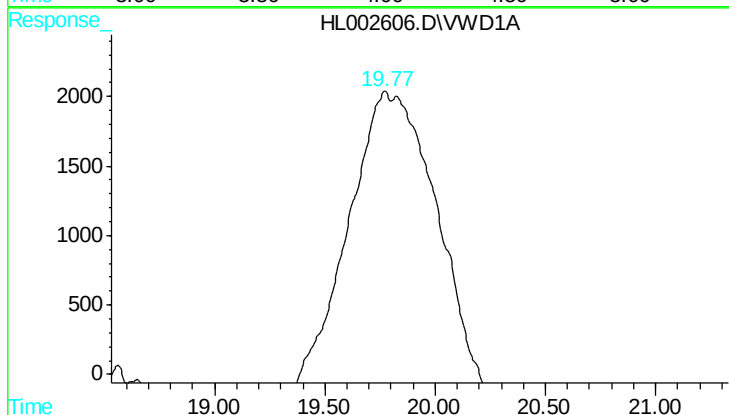

#18 PETN

R.T.: 19.773 min
Delta R.T.: -0.079 min
Response: 834503
Conc: 84.27 ug/L