

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
 Data File : HL003206.D
 Signal(s) : VWD1A.CH
 Acq On : 08-Jun-2012, 07:46
 Operator : HLM
 Sample : D2921-11MS2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Integration File: events.e
 Quant Time: Jun 14 07:33:01 2012
 Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL060712.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Wed Jun 13 15:12:30 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.341	867304	238.475 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 79.49%
Target Compounds			
2) T HMX	0.897	960047	207.233 ug/L
3) T RDX	1.726	10036025	1767.212 ug/L
8) T 4-Amino-2,6-dinitroto...	7.222f	170133	22.544 ug/L
9) T 2,4-Dinitrotoluene	8.058f	5145821	324.909 ug/L
16) T 3,5-Dinitroaniline	3.872f	131839	6.932 ug/L
17) T Nitroglycerin	6.059	286877	4821.922 ug/L


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
Data File : HL003206.D
Signal(s) : VWD1A.CH
Acq On : 08-Jun-2012, 07:46
Operator : HLM
Sample : D2921-11MS2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: events.e
Quant Time: Jun 14 07:33:01 2012
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jun 13 15:12:30 2012
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

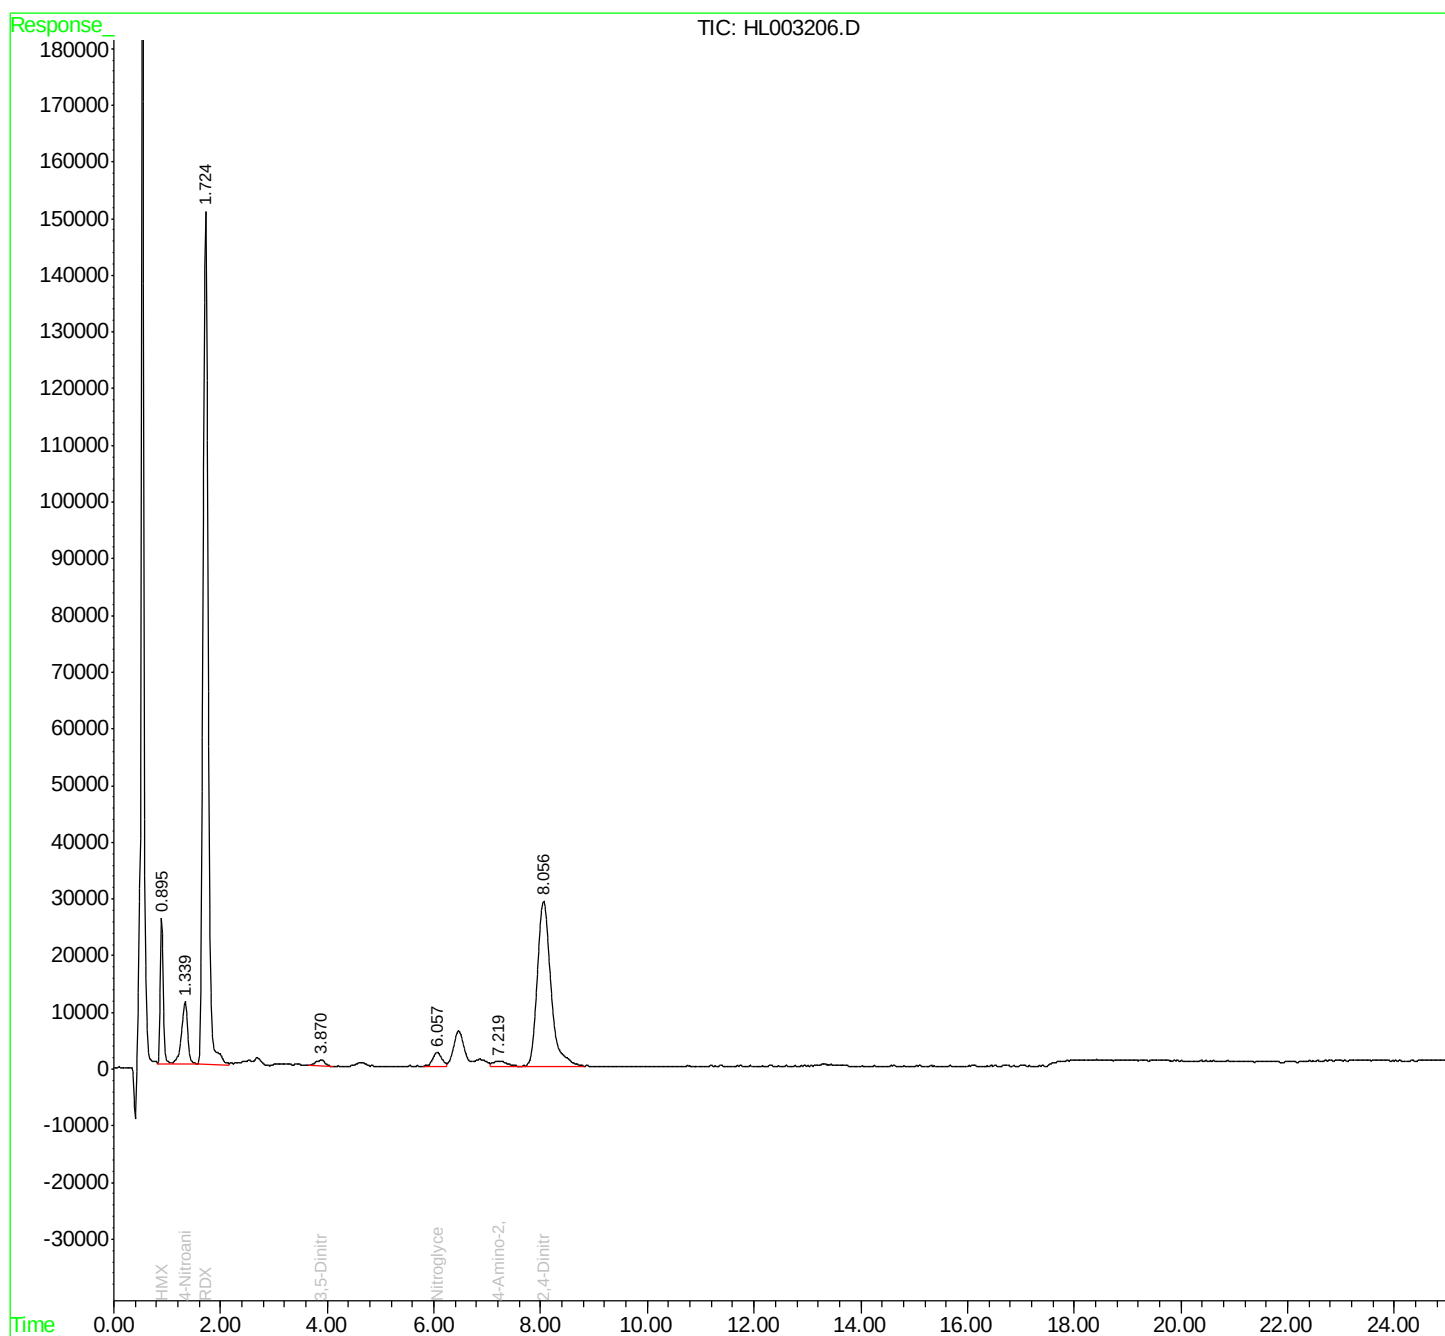

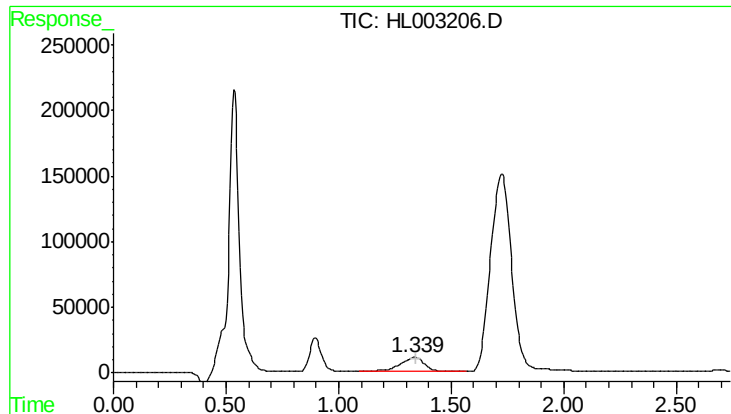


#1 4-Nitroaniline

R.T.: 1.341 min
Delta R.T.: -0.005 min
Response: 867304
Conc: 238.48 ug/L

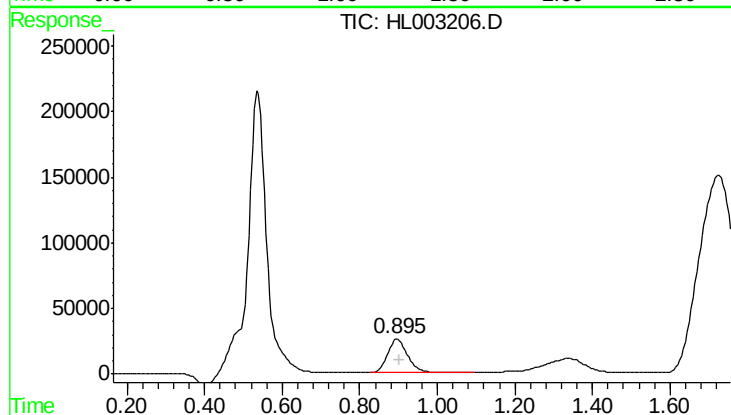


#2 HMX

R.T.: 0.897 min
Delta R.T.: -0.005 min
Response: 960047
Conc: 207.23 ug/L

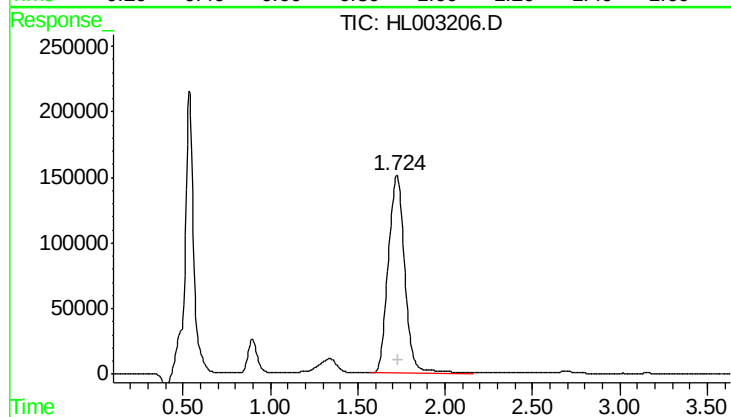


#3 RDX

R.T.: 1.726 min
Delta R.T.: -0.009 min
Response: 10036025
Conc: 1767.21 ug/L

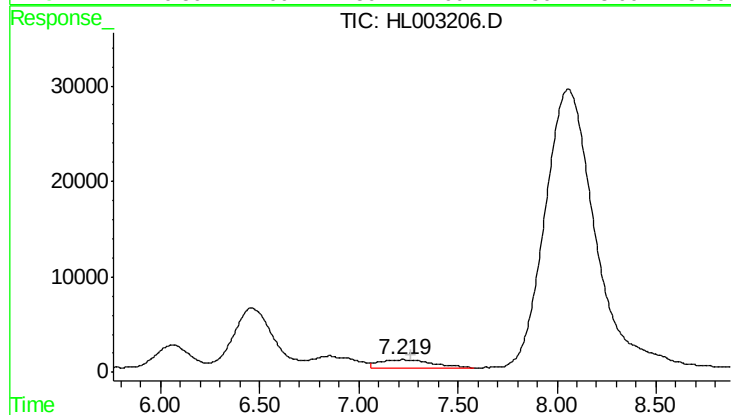


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.222 min
Delta R.T.: -0.042 min
Response: 170133
Conc: 22.54 ug/L

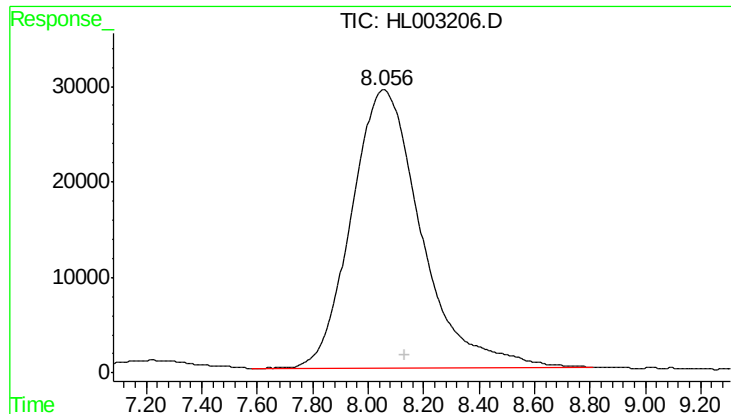


#9 2,4-Dinitrotoluene

R.T.: 8.058 min
Delta R.T.: -0.074 min
Response: 5145821
Conc: 324.91 ug/L

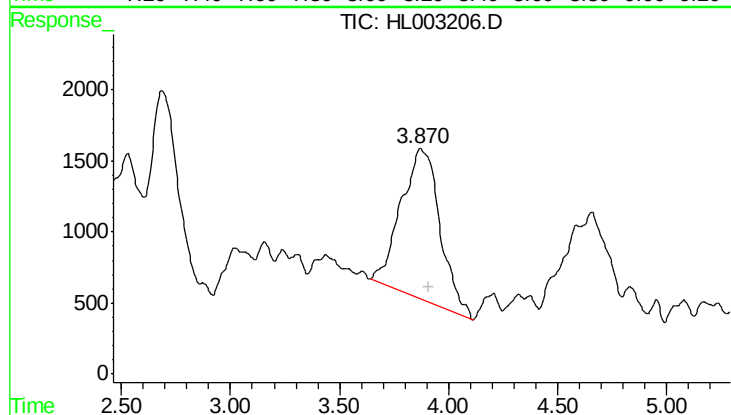

#16 3,5-Dinitroaniline

R.T.: 3.872 min
Delta R.T.: -0.040 min
Response: 131839
Conc: 6.93 ug/L

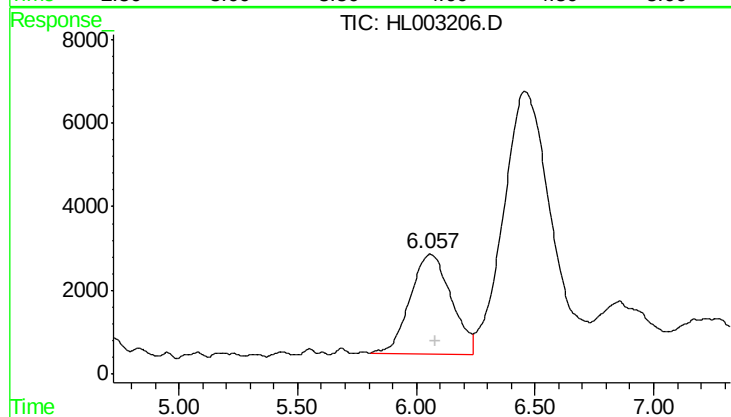

#17 Nitroglycerin

R.T.: 6.059 min
Delta R.T.: -0.020 min
Response: 286877
Conc: 4821.92 ug/L