



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
Data File : HL003173.D
Signal(s) : VWD1A.CH
Acq On : 07-Jun-2012, 16:57
Operator : HLM
Sample : ICVHL060712
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
ICVHL060712

Integration File: events.e
Quant Time: Jun 14 01:55:49 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jun 08 13:23:23 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

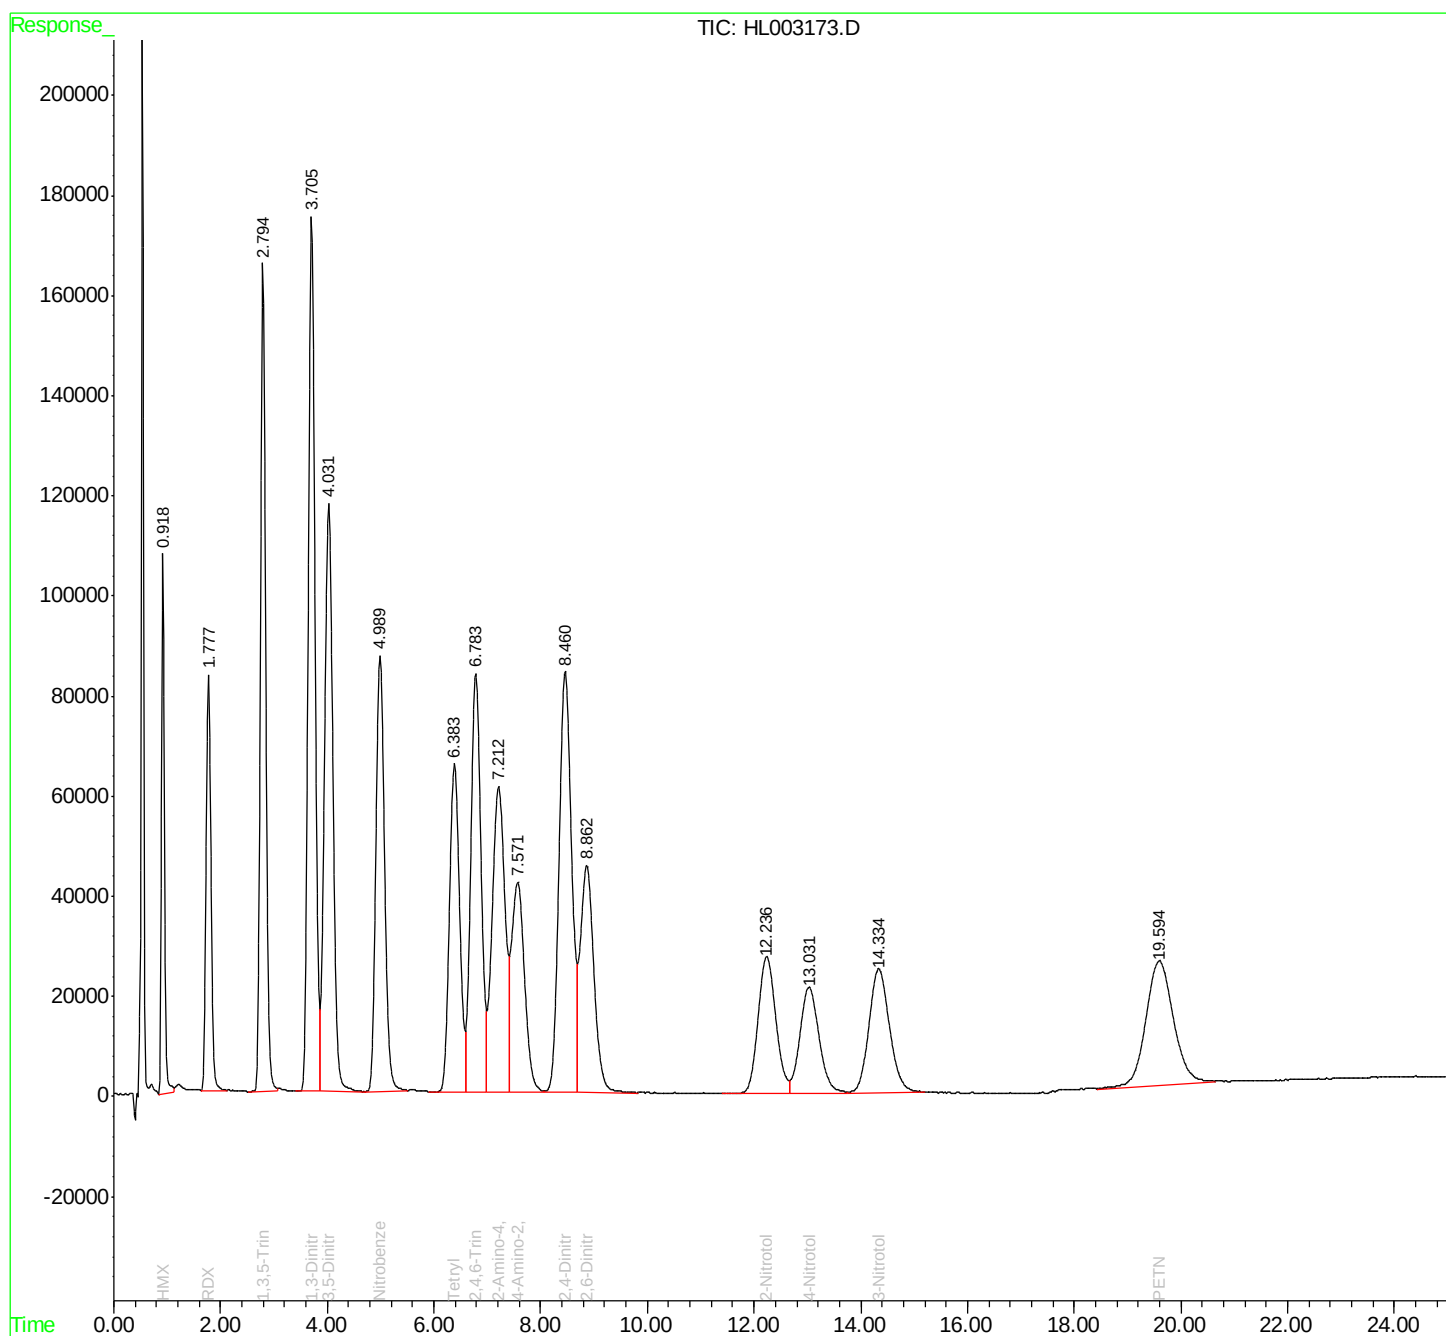


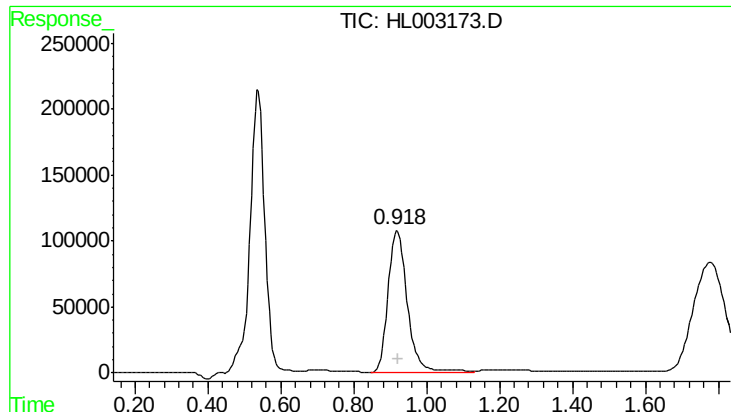

#2 HMX


R.T.: 0.920 min
Delta R.T.: -0.003 min
Response: 3931684
Conc: 899.64 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL060712

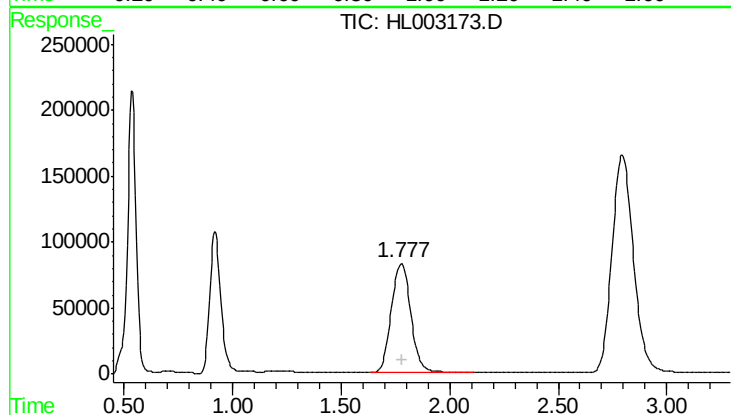


#3 RDX

R.T.: 1.779 min
Delta R.T.: -0.003 min
Response: 5177439
Conc: 911.68 ug/L

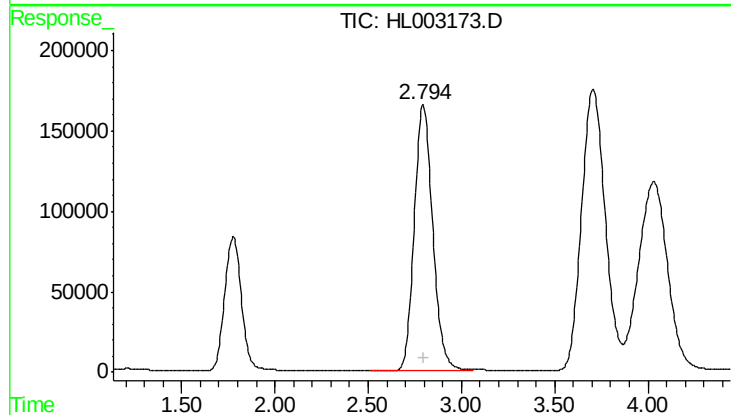


#4 1,3,5-Trinitrobenzene

R.T.: 2.796 min
Delta R.T.: -0.005 min
Response: 11380373
Conc: 932.31 ug/L

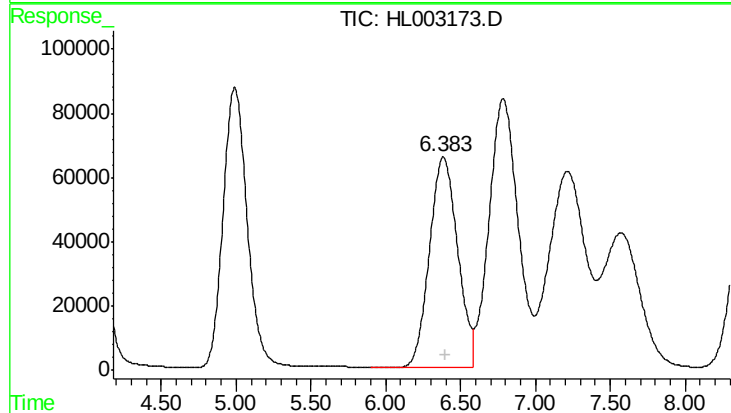

#5 Tetryl


R.T.: 6.385 min
Delta R.T.: -0.013 min
Response: 8597089
Conc: 964.26 ug/L

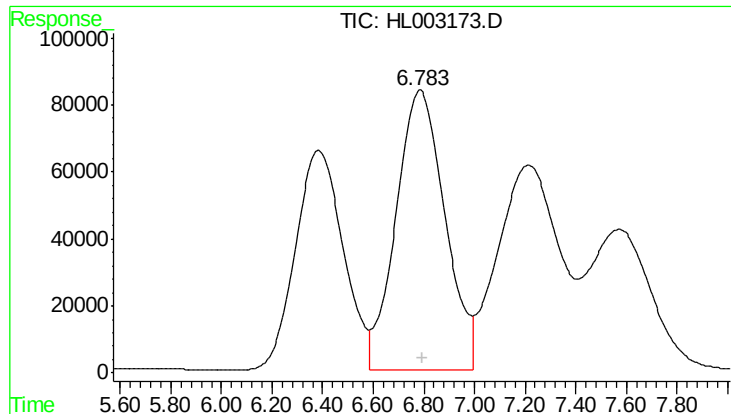

#6 2,4,6-Trinitrotoluene


R.T.: 6.785 min
Delta R.T.: -0.012 min
Response: 11222131
Conc: 952.71 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL060712

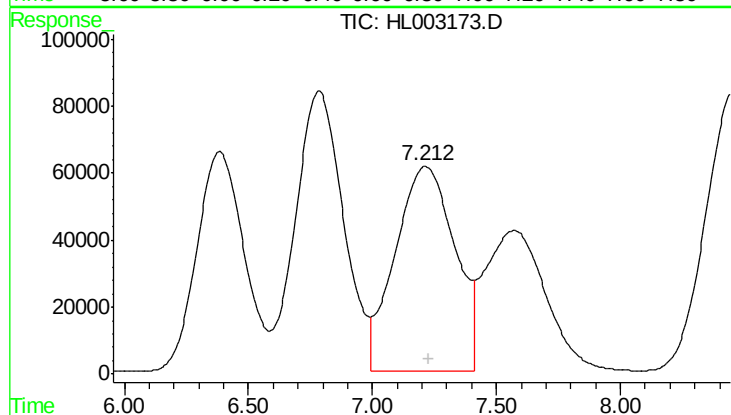


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.214 min
Delta R.T.: -0.013 min
Response: 10211090
Conc: 914.34 ug/L

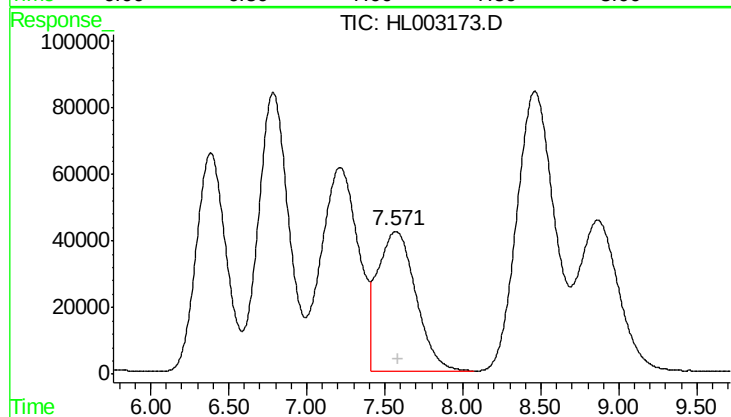


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.572 min
Delta R.T.: -0.015 min
Response: 7231177
Conc: 958.19 ug/L

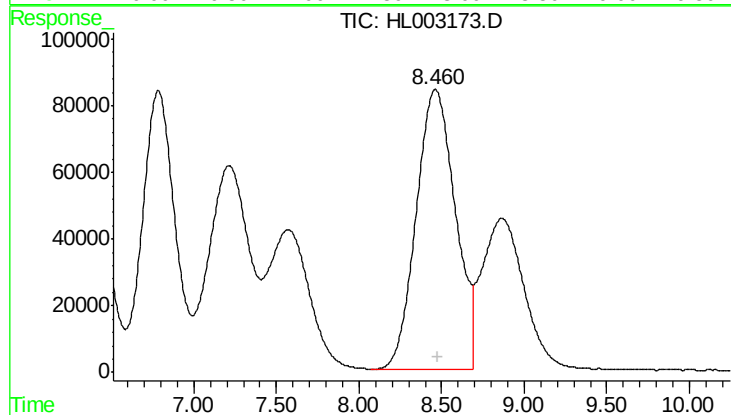

#9 2,4-Dinitrotoluene


R.T.: 8.462 min
Delta R.T.: -0.014 min
Response: 13916830
Conc: 878.71 ug/L

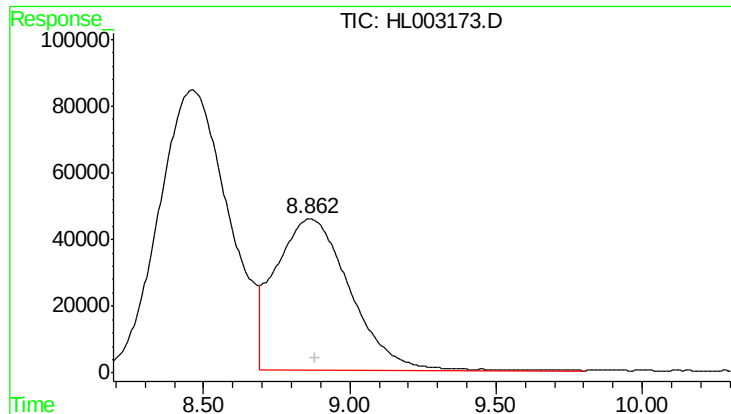

#10 2,6-Dinitrotoluene


R.T.: 8.865 min
Delta R.T.: -0.016 min
Response: 8133867
Conc: 924.08 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL060712

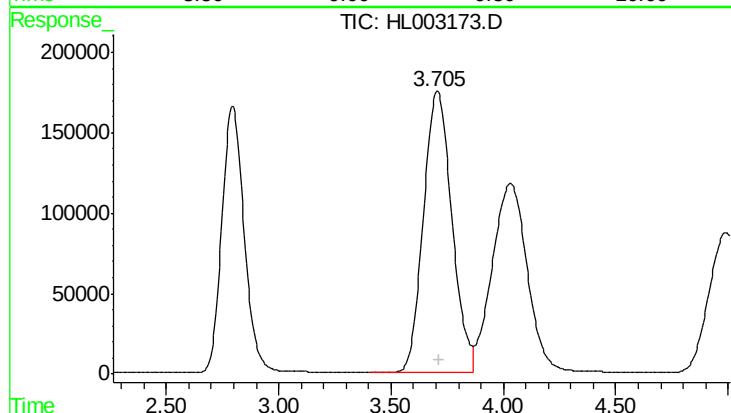


#11 1,3-Dinitrobenzene

R.T.: 3.707 min
Delta R.T.: -0.007 min
Response: 15392481
Conc: 926.95 ug/L

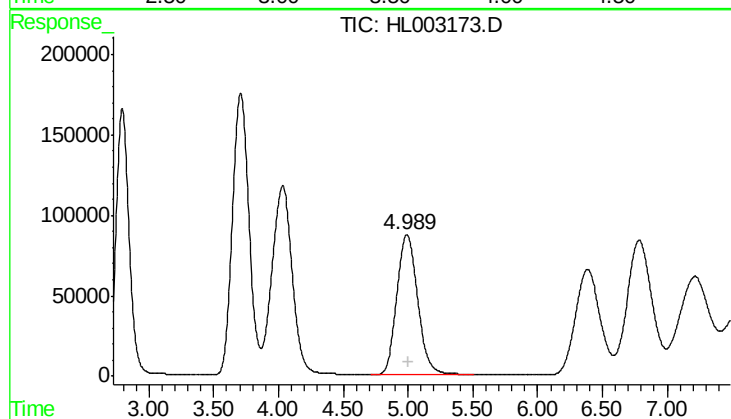


#12 Nitrobenzene

R.T.: 4.992 min
Delta R.T.: -0.009 min
Response: 9684932
Conc: 864.68 ug/L

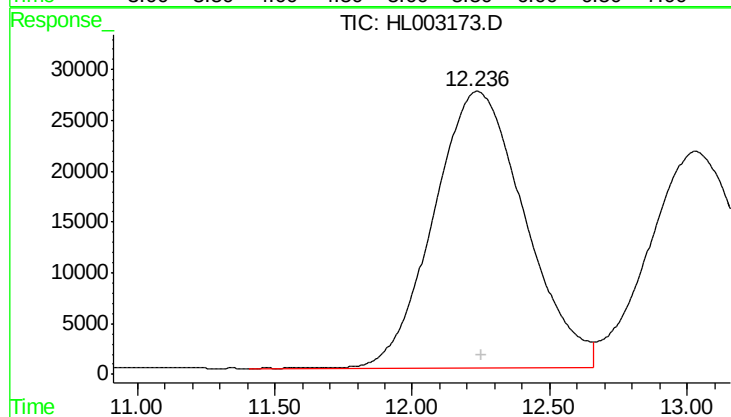

#13 2-Nitrotoluene


R.T.: 12.238 min
Delta R.T.: -0.016 min
Response: 6320477
Conc: 906.09 ug/L

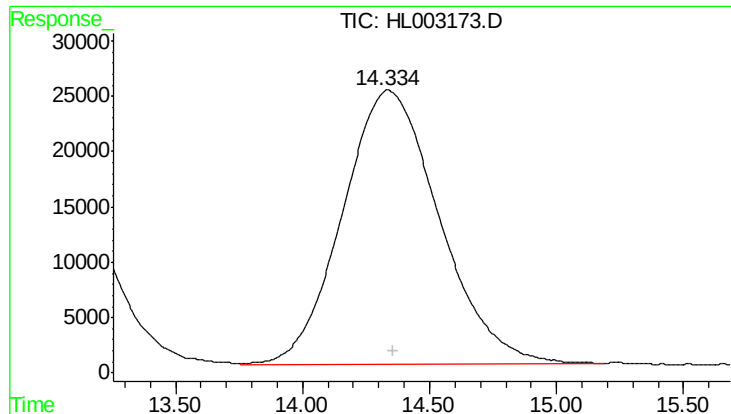

#14 3-Nitrotoluene


R.T.: 14.338 min
Delta R.T.: -0.021 min
Response: 6584589
Conc: 891.68 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL060712

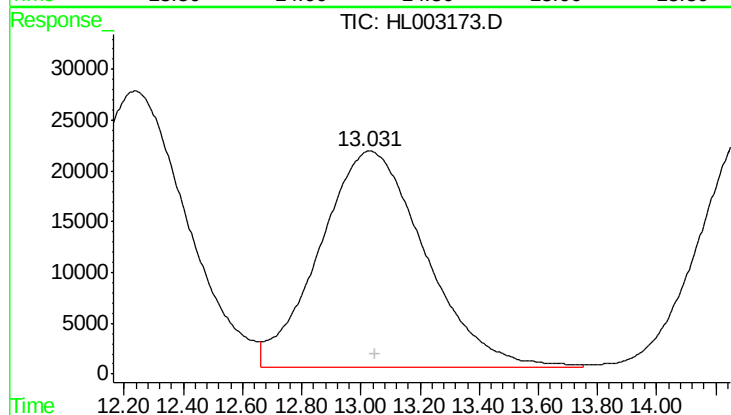


#15 4-Nitrotoluene

R.T.: 13.033 min
Delta R.T.: -0.016 min
Response: 5289433
Conc: 889.60 ug/L

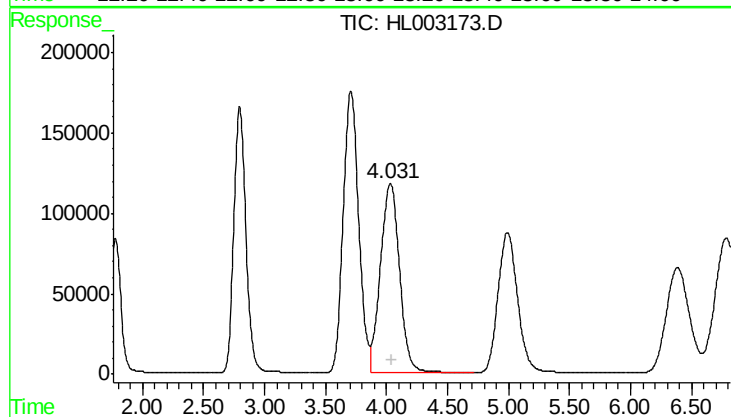

#16 3,5-Dinitroaniline

R.T.: 4.033 min
Delta R.T.: -0.011 min
Response: 12867868
Conc: 676.63 ug/L

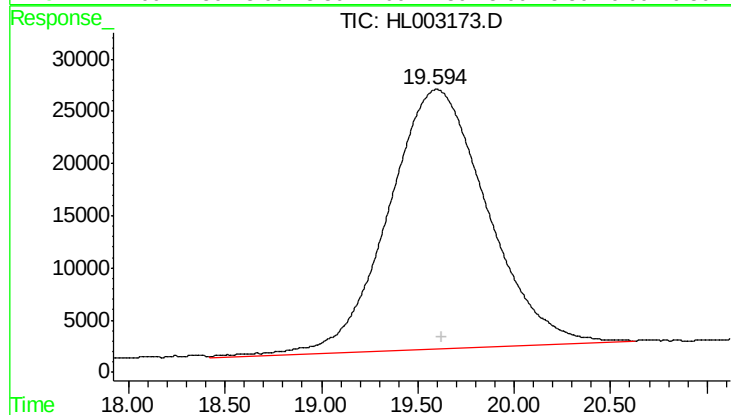

#18 PETN

R.T.: 19.599 min
Delta R.T.: -0.023 min
Response: 8867490
Conc: 920.60 ug/L

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
 Data File : HL003173.D
 Signal(s) : VWD1A.CH
 Acq On : 07-Jun-2012, 16:57
 Operator : HLM
 Sample : ICVHL060712
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL060712

Integration File: events.e
 Quant Time: Jun 14 01:55:49 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Fri Jun 08 13:23:23 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	0.920	3931684	899.635 ug/L
3) T RDX	1.779	5177439	911.679 ug/L
4) T 1,3,5-Trinitrobenzene	2.796	11380373	932.310 ug/L
5) T Tetryl	6.385	8597089	964.261 ug/L
6) T 2,4,6-Trinitrotoluene	6.785	11222131	952.711 ug/L
7) T 2-Amino-4,6-dinitroto...	7.214	10211090	914.336 ug/L
8) T 4-Amino-2,6-dinitroto...	7.572	7231177	958.185 ug/L
9) T 2,4-Dinitrotoluene	8.462	13916830	878.715 ug/L
10) T 2,6-Dinitrotoluene	8.865	8133867	924.076 ug/L
11) T 1,3-Dinitrobenzene	3.707	15392481	926.950 ug/L
12) T Nitrobenzene	4.992	9684932	864.683 ug/L
13) T 2-Nitrotoluene	12.238	6320477	906.095 ug/L
14) T 3-Nitrotoluene	14.338	6584589	891.677 ug/L
15) T 4-Nitrotoluene	13.033	5289433	889.597 ug/L
16) T 3,5-Dinitroaniline	4.033	12867868	676.628 ug/L
18) T PETN	19.599	8867490	920.600 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.