

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
Data File : HL003188.D
Signal(s) : VWD1A.CH
Acq On : 07-Jun-2012, 23:42
Operator : HLM
Sample : D2921-04
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
B1222SW-04A


Manual Integrations
APPROVED

AHPatel
6/19/2012 2:12:10 AM

Integration File: events.e
Quant Time: Jun 14 07:14:47 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jun 08 13:33:08 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

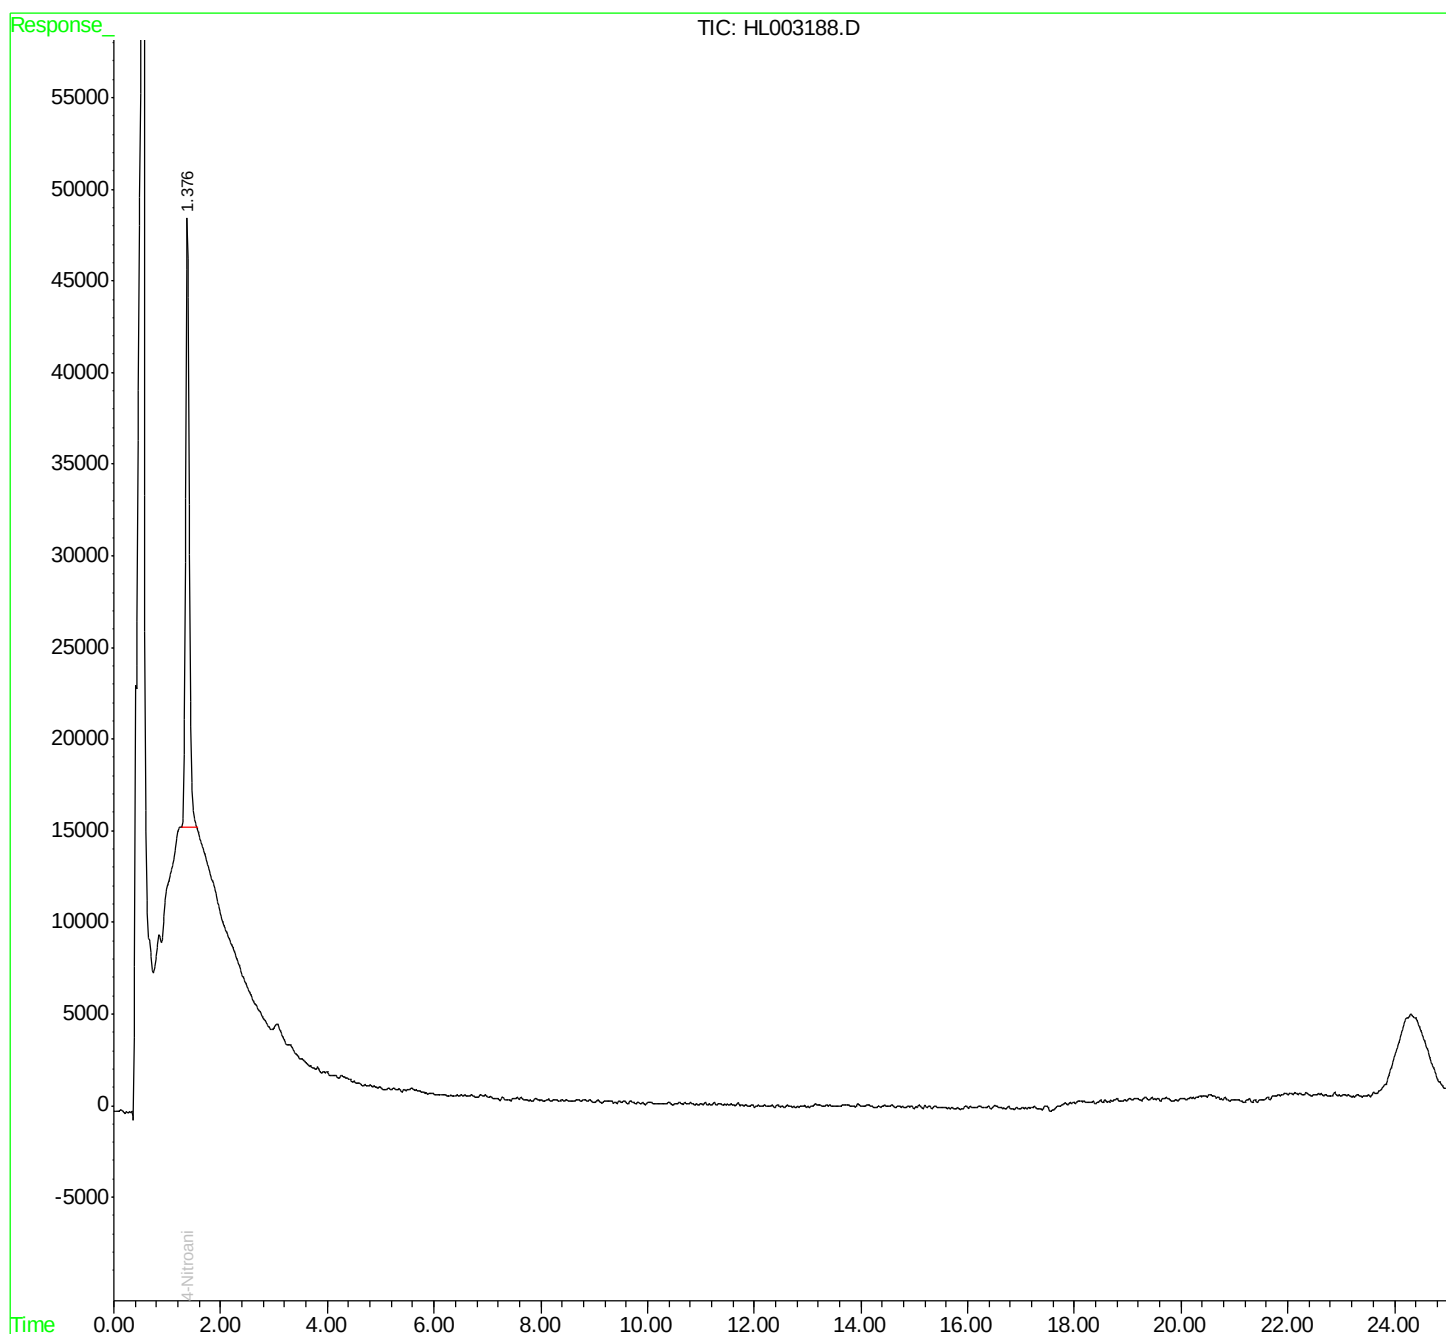

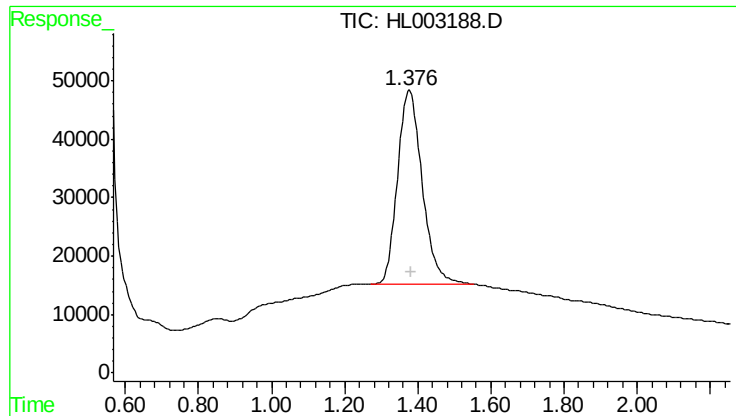

#1 4-Nitroaniline

R.T.: 1.376 min
Delta R.T.: -0.007 min
Response: 1561064
Conc: 429.23 ug/L m

Instrument :
HPLC_L
ClientSampleId :
B1222SW-04A

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:12:10 AM

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060712\
Data File : HL003188.D
Signal(s) : VWD1A.CH
Acq On : 07-Jun-2012, 23:42
Operator : HLM
Sample : D2921-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
B1222SW-04A

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:12:10 AM

Integration File: events.e
Quant Time: Jun 14 07:14:47 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jun 08 13:33:08 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.376	1561064	429.233 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery	= 143.08%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.