



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003246.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 12:46
Operator : HLM
Sample : 8330-6
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
8330-6

Integration File: events.e
Quant Time: Jun 14 05:27:47 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 16:17:29 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

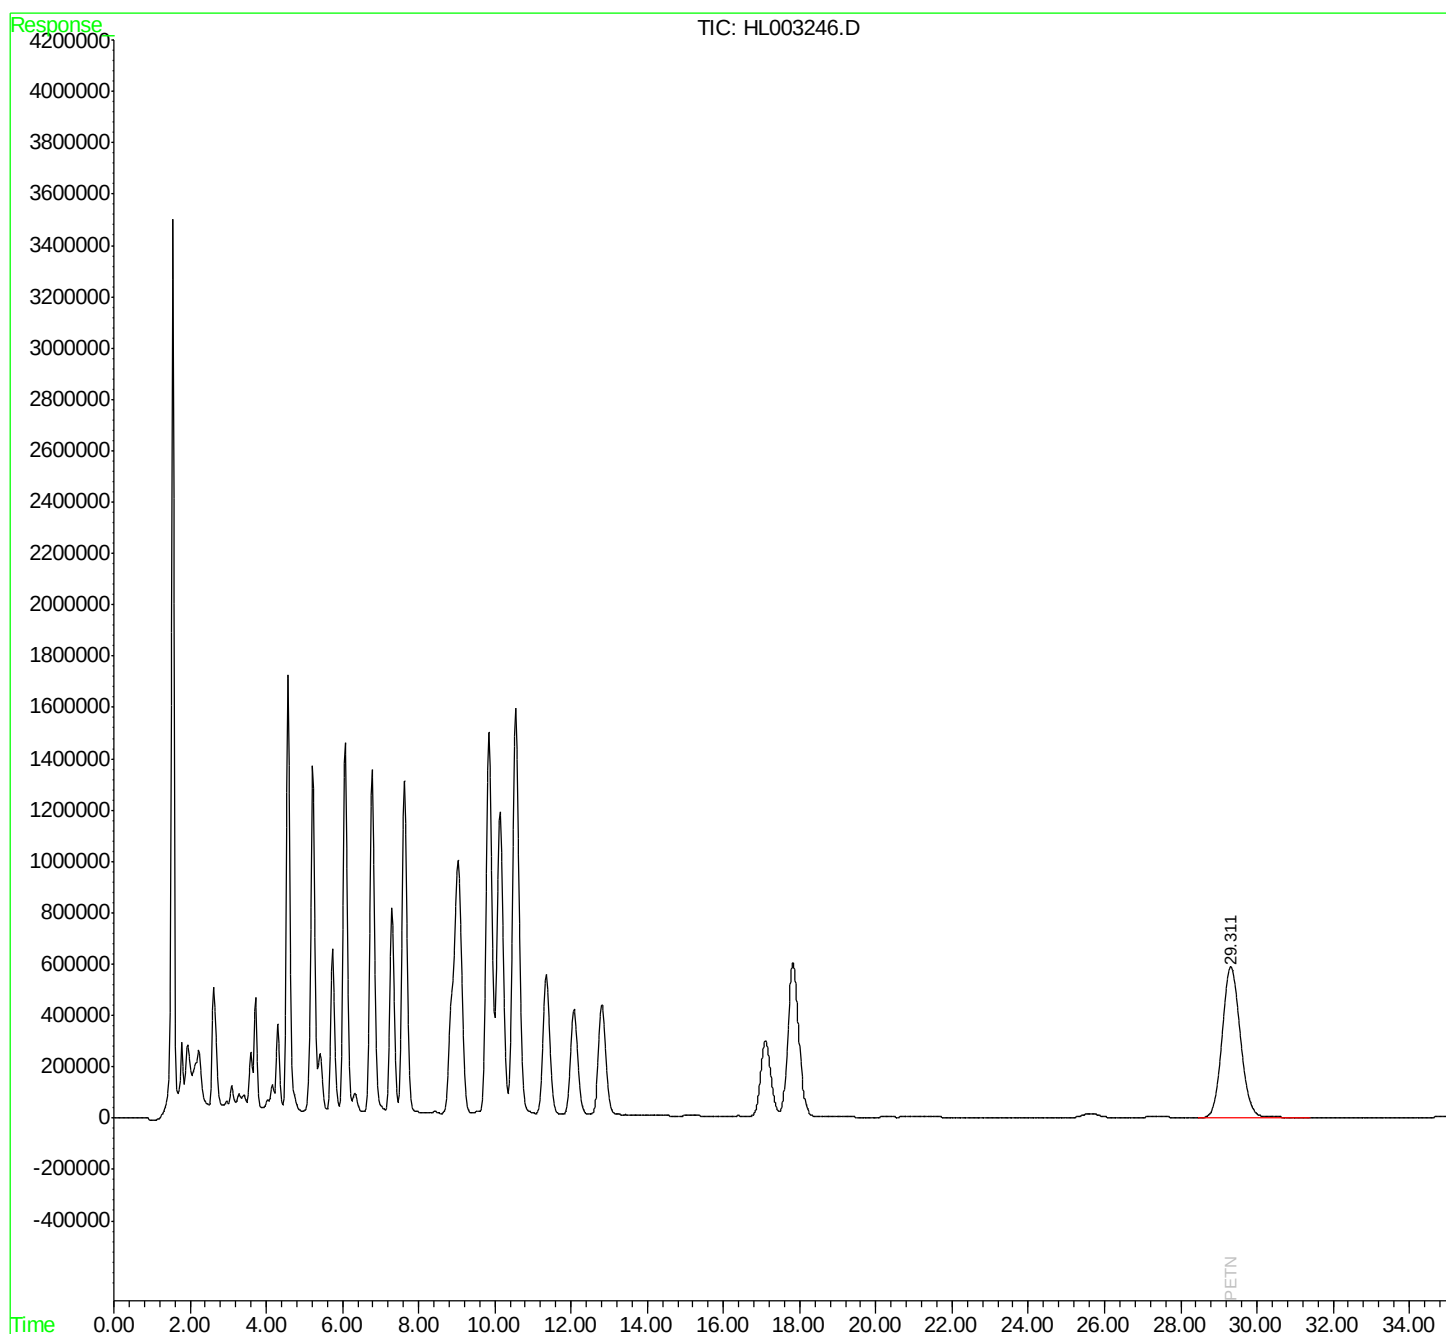

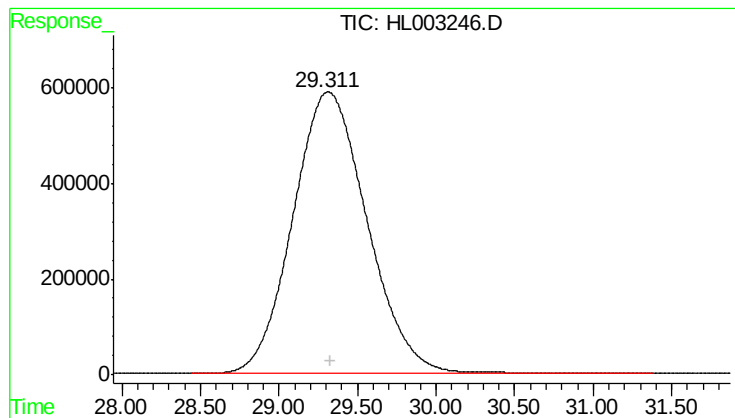

#1 PETN

R.T.: 29.313 min
Delta R.T.: -0.012 min
Response: 193917838
Conc: 2439.49 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-6

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003246.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 12:46
Operator : HLM
Sample : 8330-6
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
8330-6

Integration File: events.e
Quant Time: Jun 14 05:27:47 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 16:17:29 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

Target Compounds			
1) T PETN	29.313	193917838	2439.489 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.