

Data Path : S:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003254.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 17:42
Operator : HLM
Sample : D2921-06RE1
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE1


Manual Integrations
APPROVED

AHPatel
6/19/2012 2:21:08 AM

Integration File: events.e
Quant Time: Jun 14 05:28:15 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 18:25:04 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

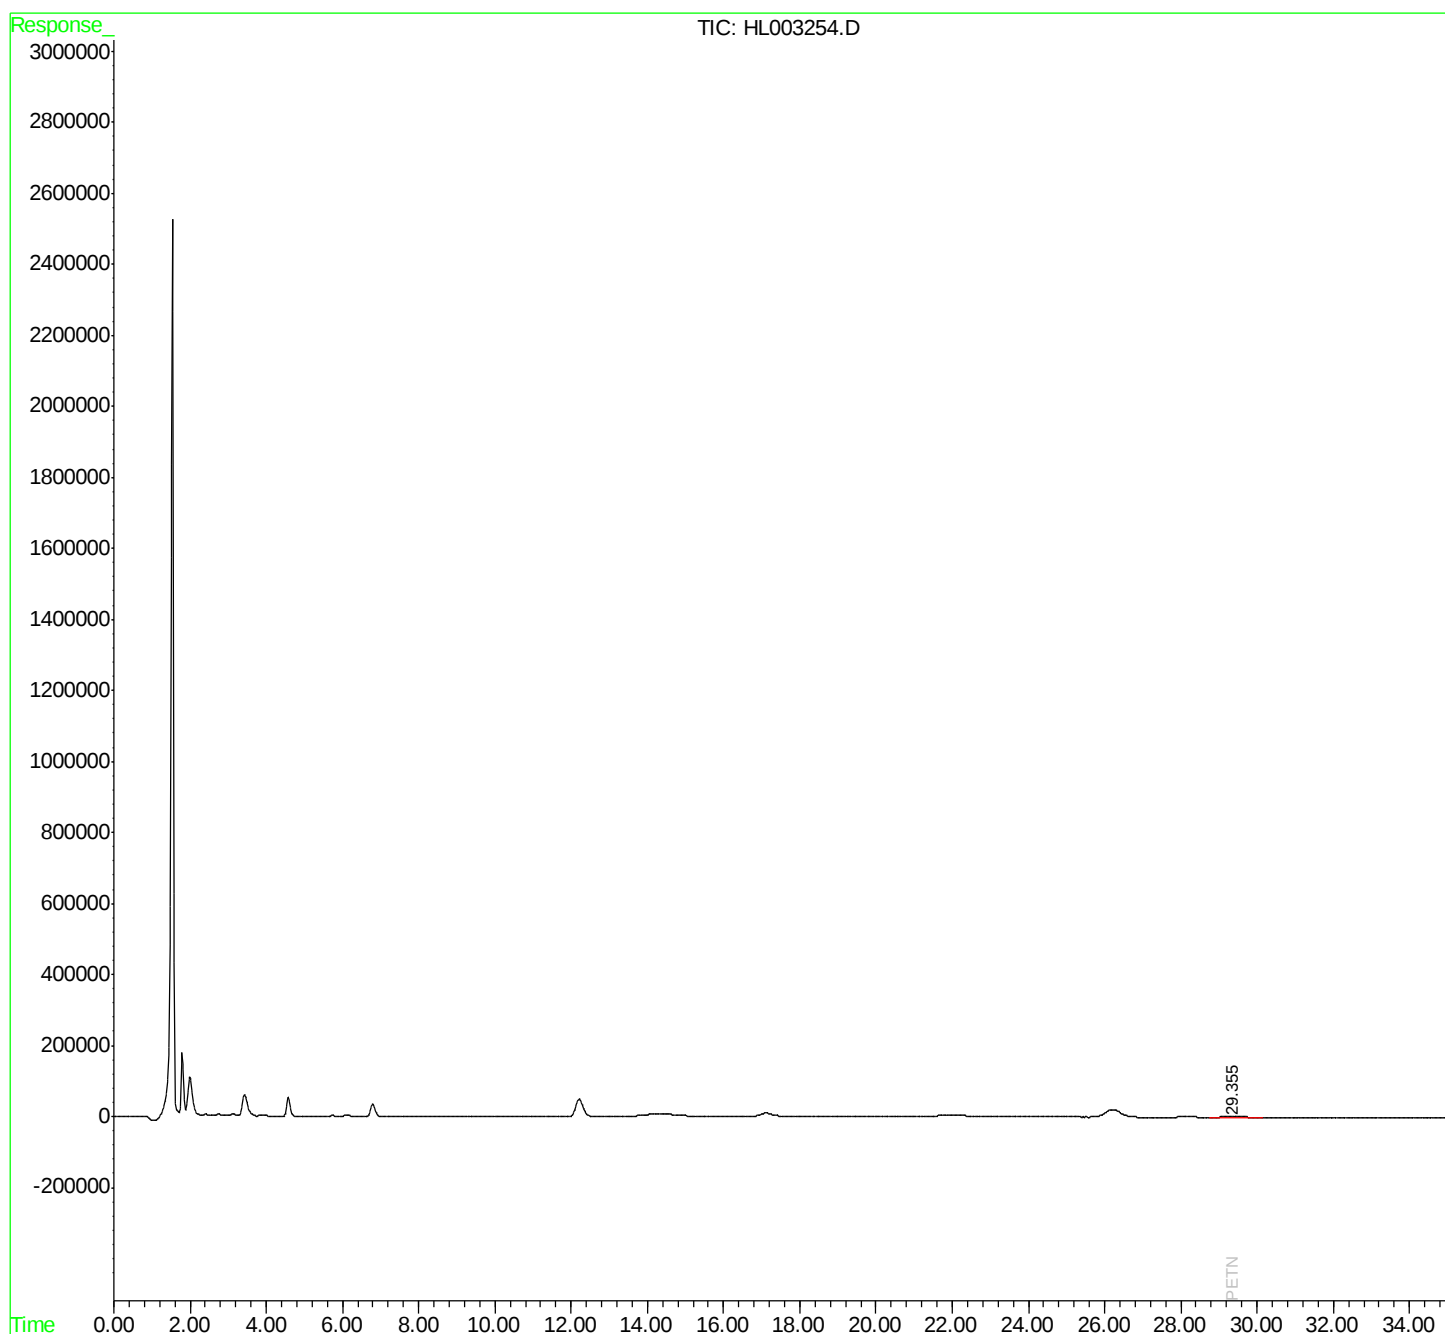

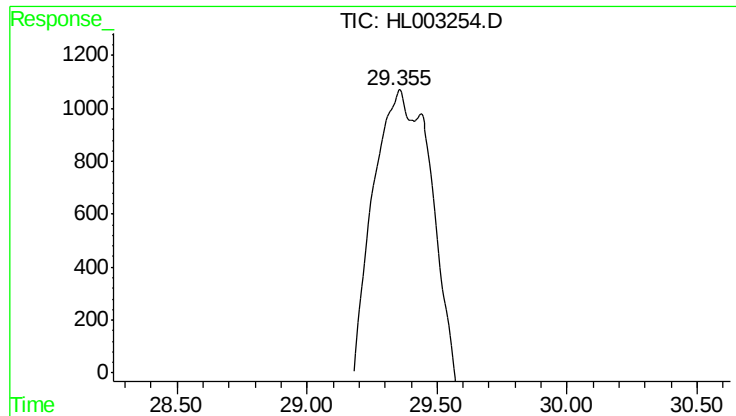

#1 PETN

R.T.: 29.355 min
Delta R.T.: 0.031 min
Response: 1209248
Conc: 71.05 ug/L m

Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE1

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:21:08 AM

Data Path : S:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003254.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 17:42
Operator : HLM
Sample : D2921-06RE1
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE1

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:21:08 AM

Integration File: events.e
Quant Time: Jun 14 05:28:15 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 18:25:04 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

Target Compounds			
1) T PETN	29.355	1209248	71.049 ug/L m

(f)=RT Delta > 1/2 Window

(m)=manual int.