



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003256.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 18:55
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
CCAL01

Integration File: events.e
Quant Time: Jun 14 05:28:22 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 18:25:04 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

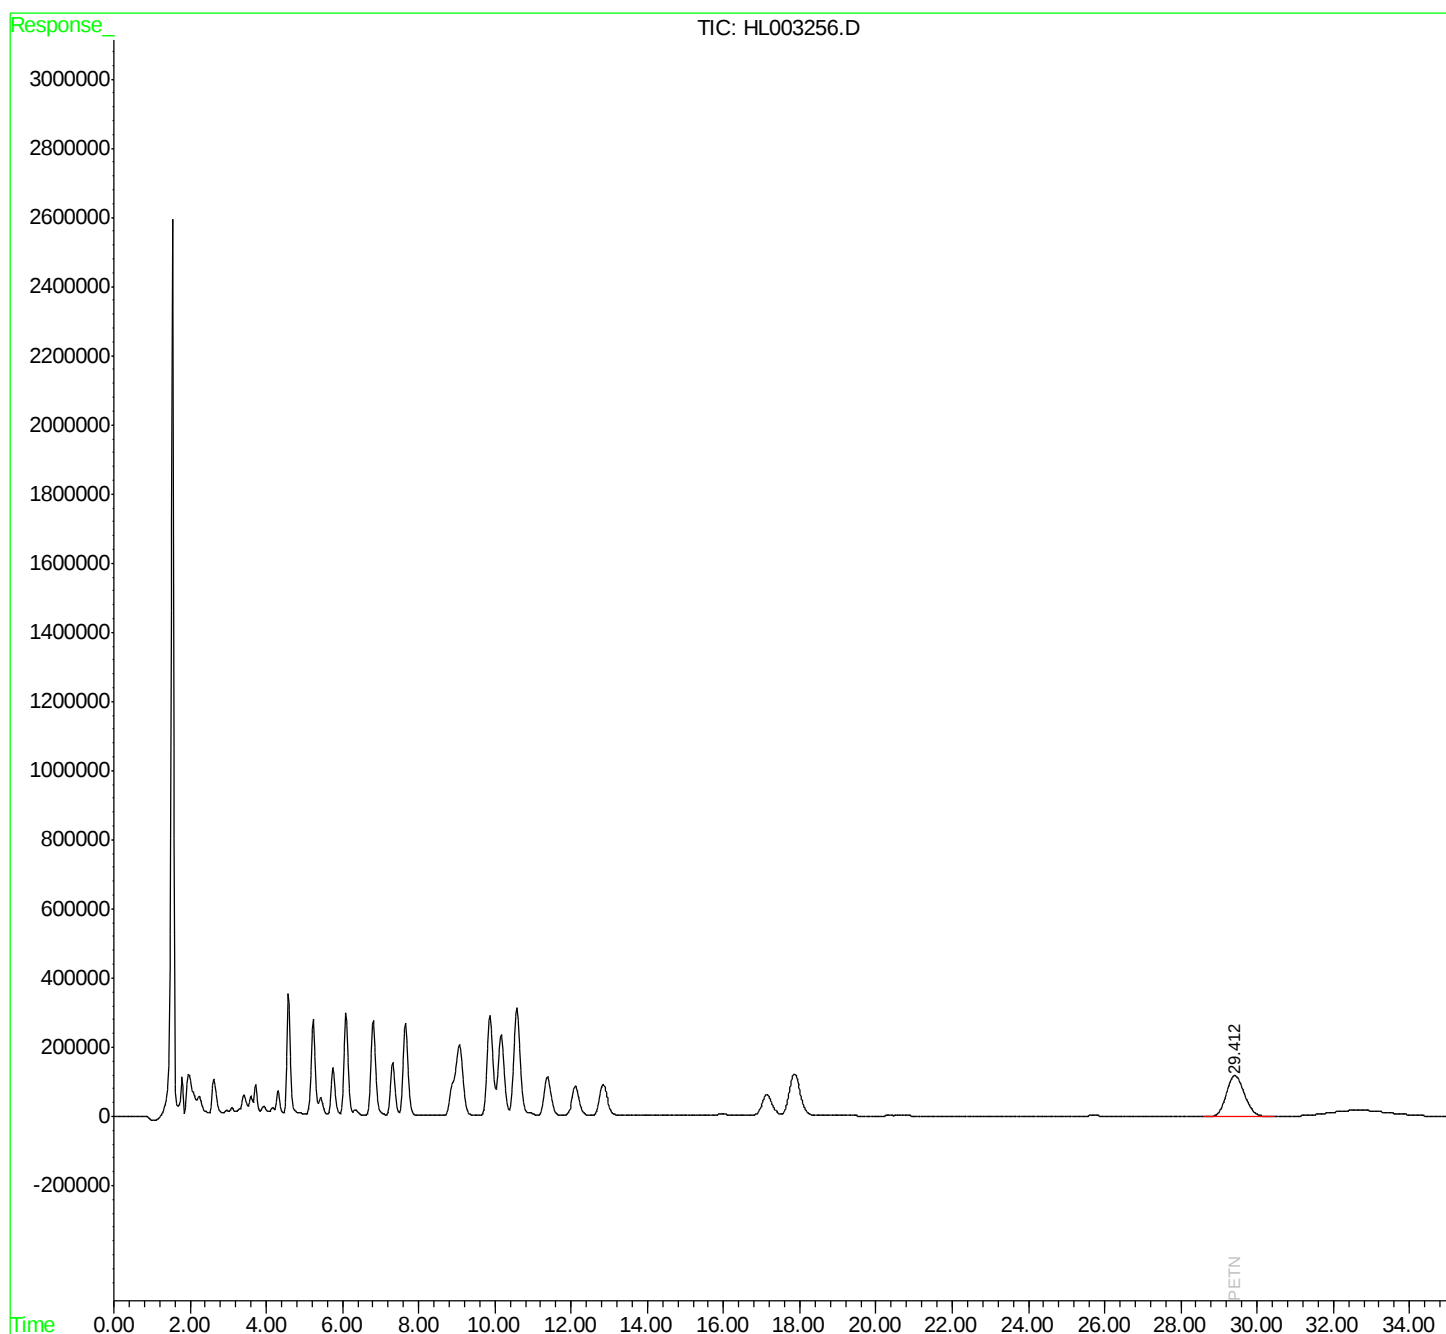

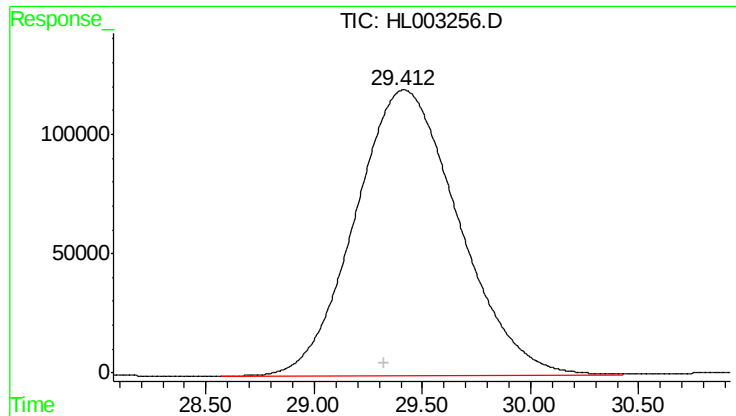

#1 PETN

R.T.: 29.415 min
Delta R.T.: 0.091 min
Response: 39893471
Conc: 2343.93 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL01

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061212\
Data File : HL003256.D
Signal(s) : VWD1A.CH
Acq On : 12-Jun-2012, 18:55
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
CCAL01

Integration File: events.e
Quant Time: Jun 14 05:28:22 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL061212.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Tue Jun 12 18:25:04 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

Target Compounds			
1) T PETN	29.415	39893471	2343.932 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.