

Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
Data File : HL003314.D
Signal(s) : VWD1A.CH
Acq On : 25-Jun-2012, 13:41
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Jun 28 04:18:20 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jun 13 15:12:30 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
6) T	2,4,6-Trinitrotoluene	6.540	8829397	749.578 ug/L
7) T	2-Amino-4,6-dinitroto...	6.883f	5888691	527.293 ug/L
15) T	4-Nitrotoluene	12.445	6774734	1139.401 ug/L
18) T	PETN	18.693	102760	10.668 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
Data File : HL003314.D
Signal(s) : VWD1A.CH
Acq On : 25-Jun-2012, 13:41
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Jun 28 04:18:20 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jun 13 15:12:30 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

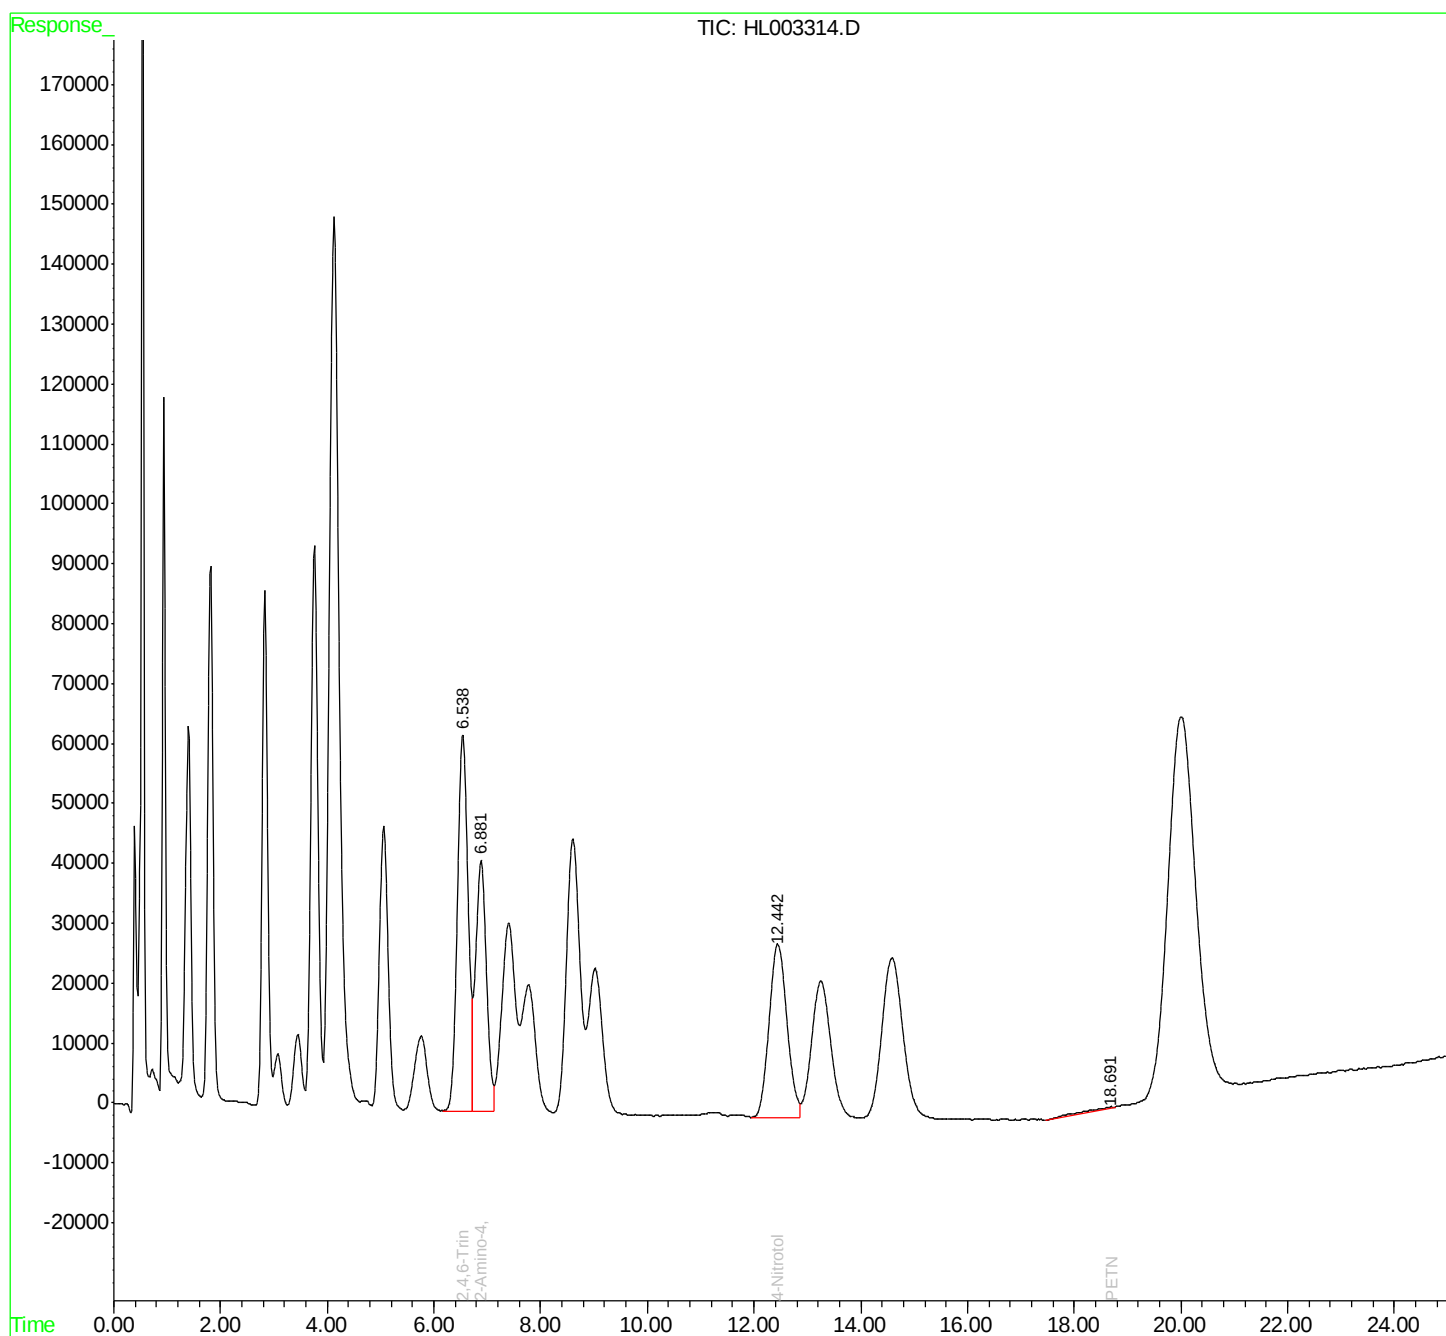


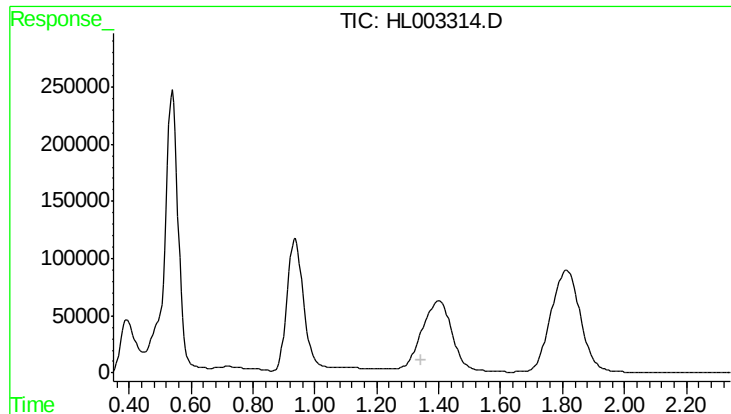

#1 4-Nitroaniline


R.T.: 0.000 min
 Exp R.T.: 1.346 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

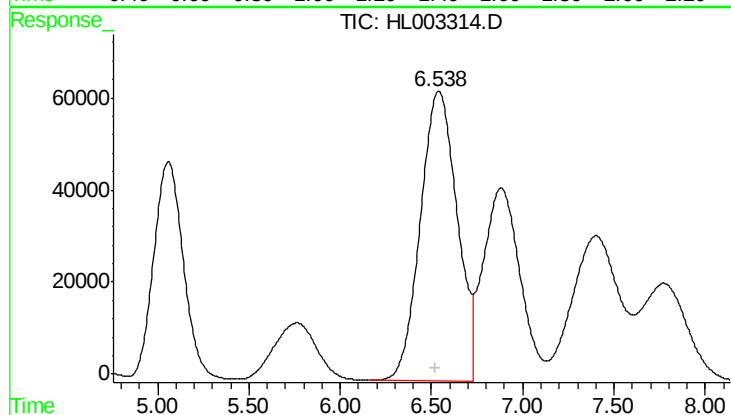


#6 2,4,6-Trinitrotoluene

R.T.: 6.540 min
 Delta R.T.: 0.017 min
 Response: 8829397
 Conc: 749.58 ug/L

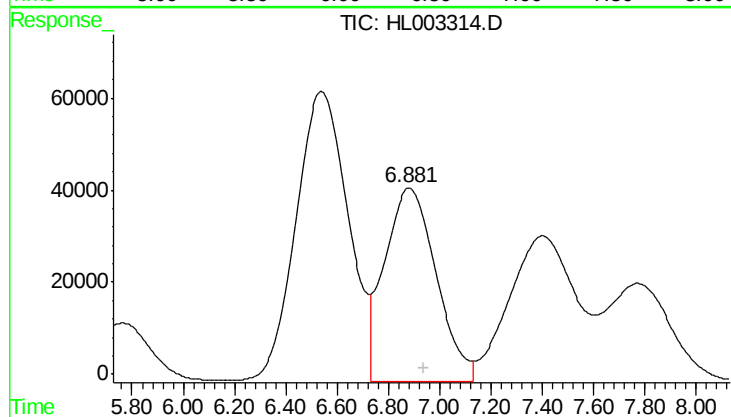


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.883 min
 Delta R.T.: -0.054 min
 Response: 5888691
 Conc: 527.29 ug/L

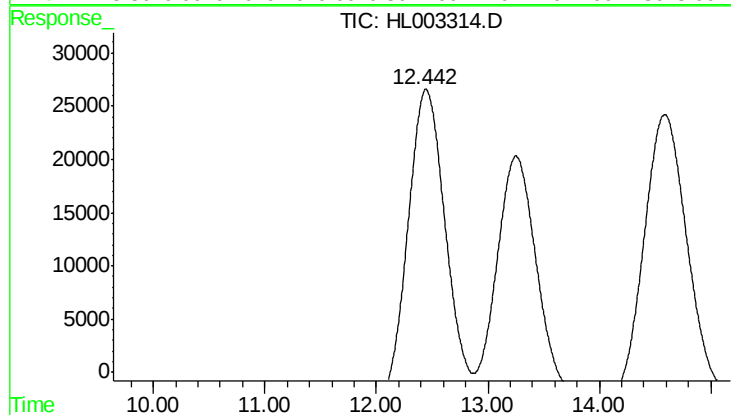

#15 4-Nitrotoluene

R.T.: 12.445 min
 Delta R.T.: -0.043 min
 Response: 6774734
 Conc: 1139.40 ug/L

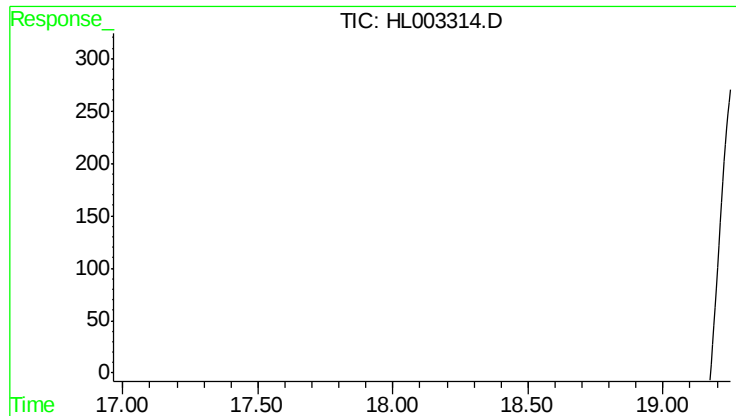

#18 PETN

R.T.: 18.693 min
Delta R.T.: -0.027 min
Response: 102760
Conc: 10.67 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV