

Data Path : S:\HPCHEM1\HPLC\_L\Data\HL062512\  
Data File : HL003319.D  
Signal(s) : VWD1A.CH  
Acq On : 25-Jun-2012, 16:04  
Operator : HLM  
Sample : PB63864BSD1  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
PB63864BSD1

Manual Integrations  
APPROVED

AHPatel  
6/29/2012 11:37:01 PM

Integration File: events.e  
Quant Time: Jun 28 04:24:33 2012  
Quant Method : S:\HPCHEM1\HPLC\_L\methods\HL060712.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Wed Jun 13 15:12:30 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| Target Compounds              |        |          |              |
| 6) T 2,4,6-Trinitrotoluene    | 6.572f | 1559967  | 132.435 ug/L |
| 7) T 2-Amino-4,6-dinitroto... | 6.921  | 3262746  | 292.157 ug/L |
| 15) T 4-Nitrotoluene          | 12.513 | 1647959  | 277.160 ug/L |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : S:\HPCHEM1\HPLC\_L\Data\HL062512\  
Data File : HL003319.D  
Signal(s) : VWD1A.CH  
Acq On : 25-Jun-2012, 16:04  
Operator : HLM  
Sample : PB63864BSD1  
Misc :  
ALS Vial : 14 Sample Multiplier: 1


Instrument :  
HPLC\_L  
ClientSampleId :  
PB63864BSD1


Manual Integrations  
APPROVED

AHPatel  
6/29/2012 11:37:01 PM

Integration File: events.e  
Quant Time: Jun 28 04:24:33 2012  
Quant Method : S:\HPCHEM1\HPLC\_L\methods\HL060712.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Wed Jun 13 15:12:30 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

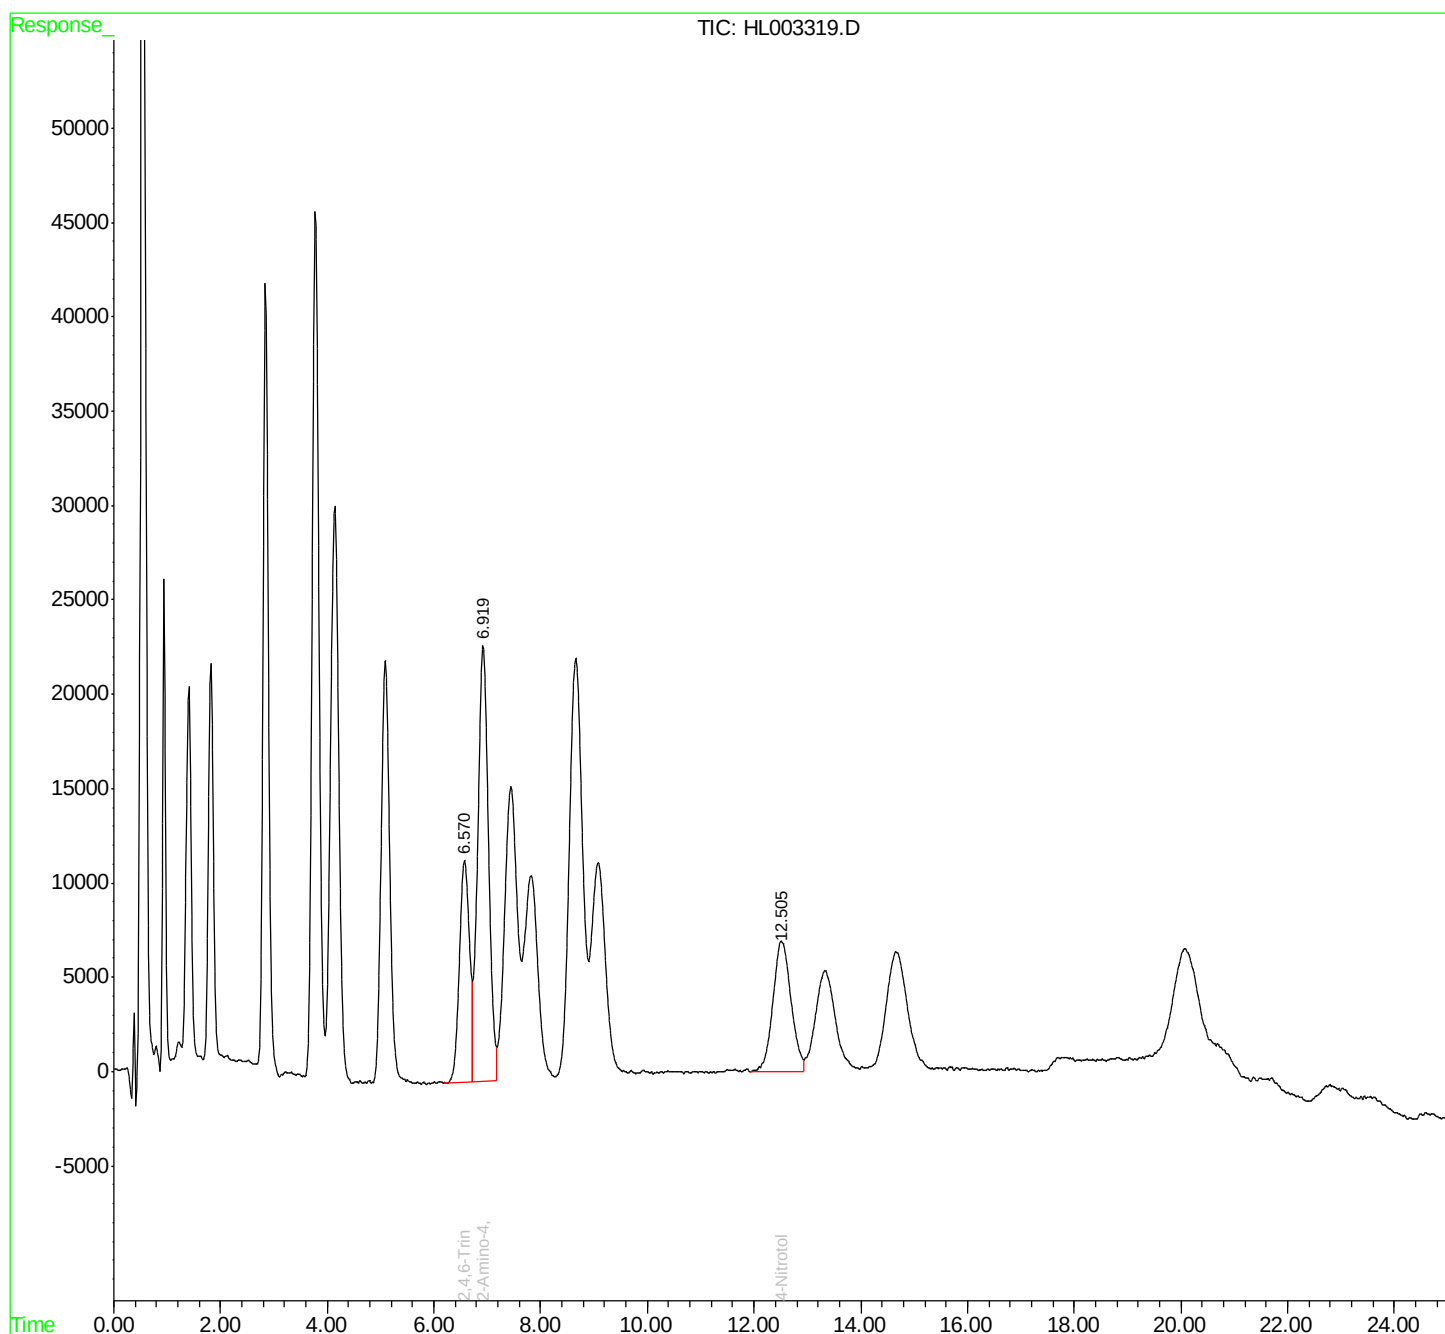

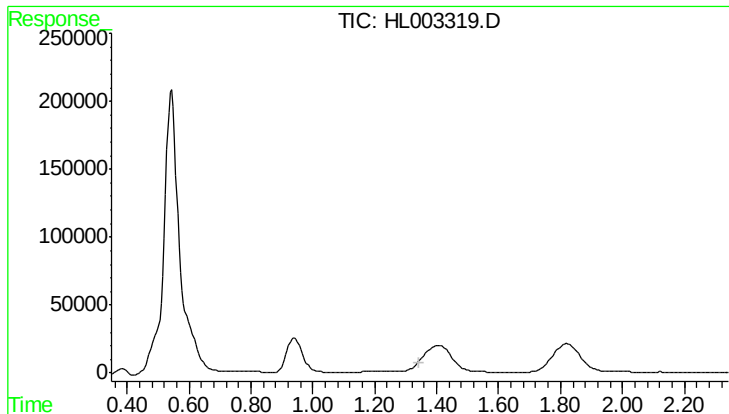


#1 4-Nitroaniline

R.T.: 0.000 min  
Exp R.T.: 1.346 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
PB63864BSD1


Manual Integrations  
APPROVED

AHPatel  
6/29/2012 11:37:01 PM

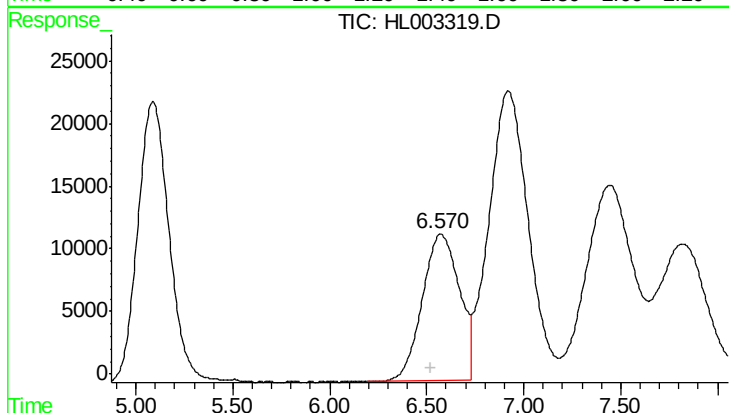


#6 2,4,6-Trinitrotoluene

R.T.: 6.572 min  
Delta R.T.: 0.049 min  
Response: 1559967  
Conc: 132.43 ug/L

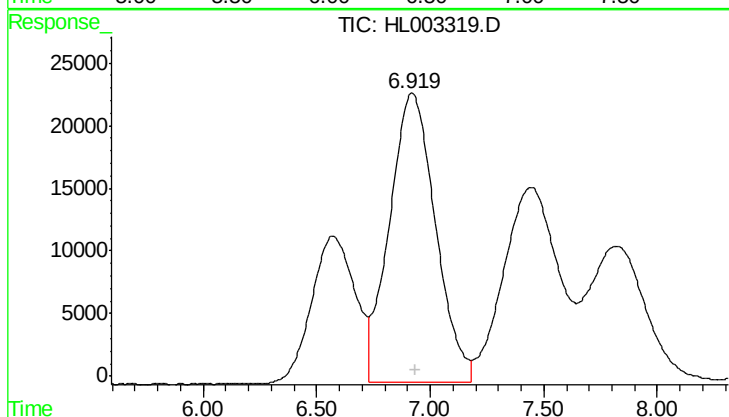

#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.921 min  
Delta R.T.: -0.016 min  
Response: 3262746  
Conc: 292.16 ug/L

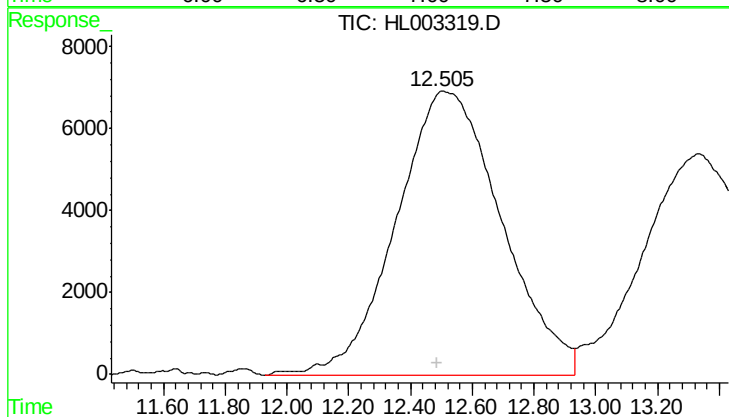

#15 4-Nitrotoluene

R.T.: 12.513 min  
Delta R.T.: 0.026 min  
Response: 1647959  
Conc: 277.16 ug/L