

Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
Data File : HL003316.D
Signal(s) : VWD1A.CH
Acq On : 25-Jun-2012, 14:43
Operator : HLM
Sample : PB63864BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
PB63864BL

Manual Integrations
APPROVED

AHPatel
6/29/2012 11:36:59 PM

Integration File: events.e
Quant Time: Jun 28 03:47:42 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jun 22 17:39:50 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.398	1163118	319.813 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery	= 106.60%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
Data File : HL003316.D
Signal(s) : VWD1A.CH
Acq On : 25-Jun-2012, 14:43
Operator : HLM
Sample : PB63864BL
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
PB63864BL


Manual Integrations
APPROVED

AHPatel
6/29/2012 11:36:59 PM

Integration File: events.e
Quant Time: Jun 28 03:47:42 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Jun 22 17:39:50 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

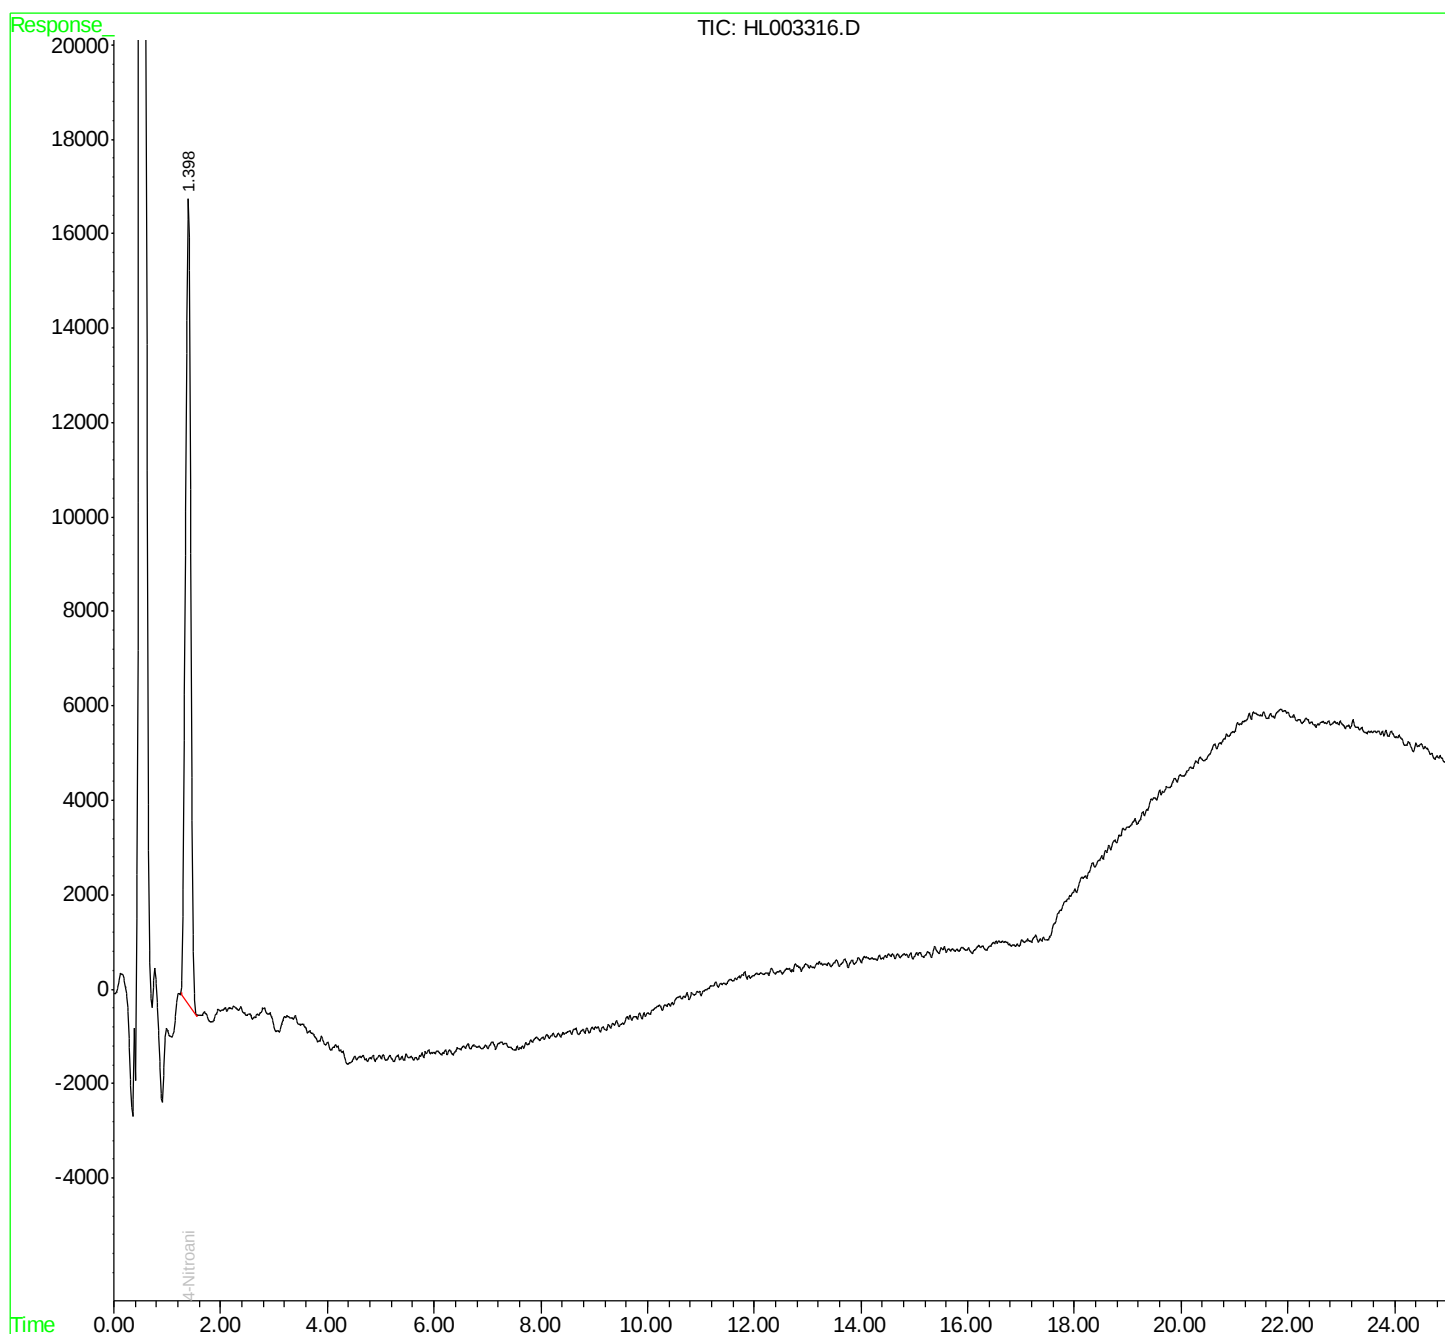

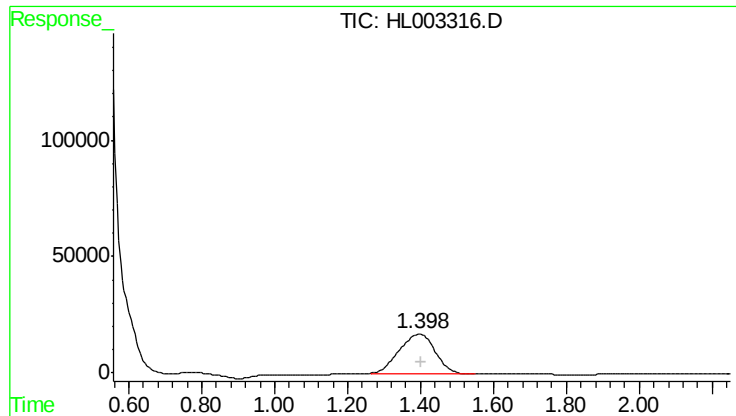

#1 4-Nitroaniline

R.T.: 1.398 min
Delta R.T.: -0.004 min
Response: 1163118
Conc: 319.81 ug/L m

Instrument :
HPLC_L
ClientSampleId :
PB63864BL

Manual Integrations
APPROVED

AHPatel
6/29/2012 11:36:59 PM