

Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
 Data File : HL003323.D
 Signal(s) : VWD1A.CH
 Acq On : 25-Jun-2012, 17:51
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Jun 28 03:47:56 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Wed Jun 13 15:12:30 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.426	4148609	1140.708 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 380.24%#
Target Compounds			
2) T HMX	0.952	4493514	969.959 ug/L
3) T RDX	1.844	6035476	1062.768 ug/L
4) T 1,3,5-Trinitrobenzene	2.873	6170308	505.488 ug/L
5) T Tetryl	6.735	9075916	1017.967 ug/L
6) T 2,4,6-Trinitrotoluene	7.089	6036103	512.439 ug/L
7) T 2-Amino-4,6-dinitroto...	7.612	5707788	511.095 ug/L
8) T 4-Amino-2,6-dinitroto...	7.993	3906201	517.601 ug/L
9) T 2,4-Dinitrotoluene	8.836	8006144	505.511 ug/L
10) T 2,6-Dinitrotoluene	9.257	4500773	511.326 ug/L
11) T 1,3-Dinitrobenzene	3.816	9089819	547.398 ug/L
12) T Nitrobenzene	5.208	5569054	497.212 ug/L
13) T 2-Nitrotoluene	12.696	6968167	998.947 ug/L
14) T 3-Nitrotoluene	14.842	7624209	1032.461 ug/L
15) T 4-Nitrotoluene	13.503	5981370	1005.970 ug/L
16) T 3,5-Dinitroaniline	4.214	20730785	1090.082 ug/L
18) T PETN	20.367	22748437	2361.685 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL062512\
Data File : HL003323.D
Signal(s) : VWD1A.CH
Acq On : 25-Jun-2012, 17:51
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Jun 28 03:47:56 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL060712.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jun 13 15:12:30 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

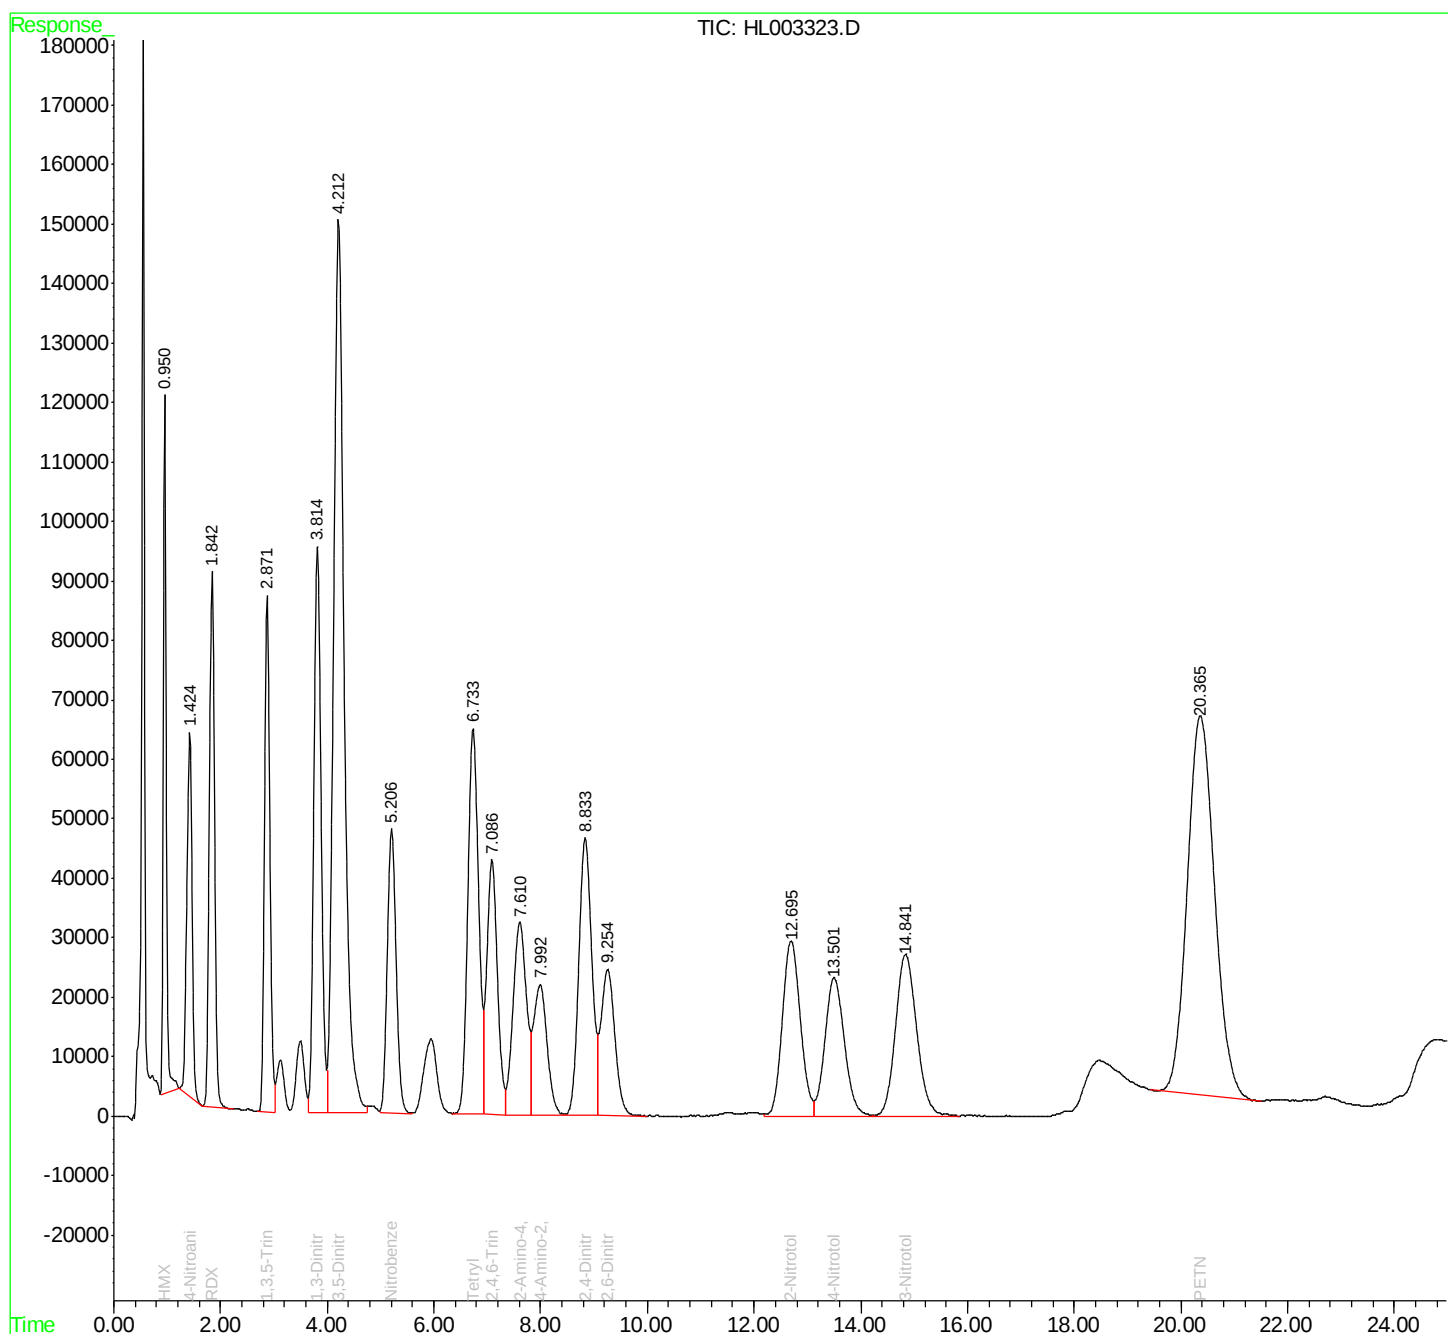


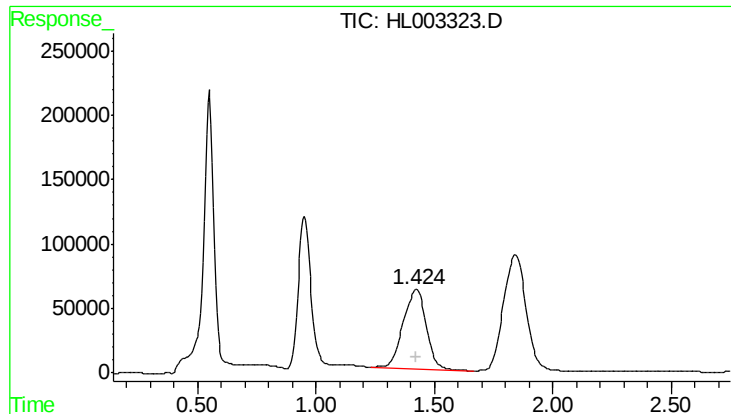

#1 4-Nitroaniline


R.T.: 1.426 min
Delta R.T.: 0.000 min
Response: 4148609
Conc: 1140.71 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

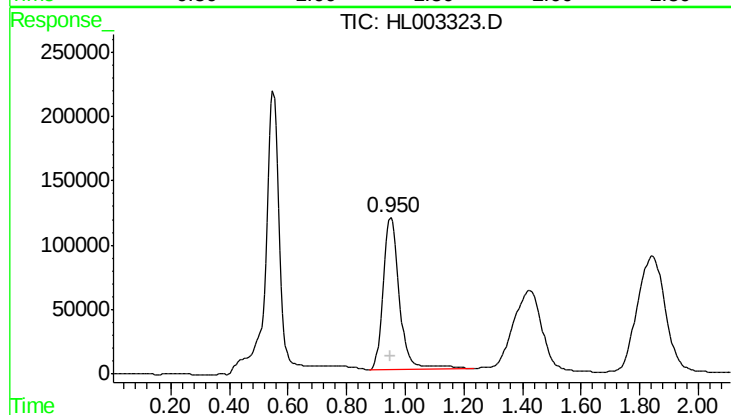


#2 HMX

R.T.: 0.952 min
Delta R.T.: 0.002 min
Response: 4493514
Conc: 969.96 ug/L

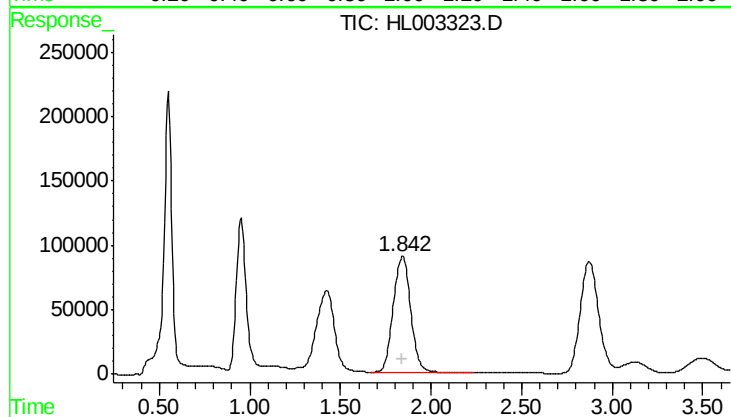


#3 RDX

R.T.: 1.844 min
Delta R.T.: 0.002 min
Response: 6035476
Conc: 1062.77 ug/L

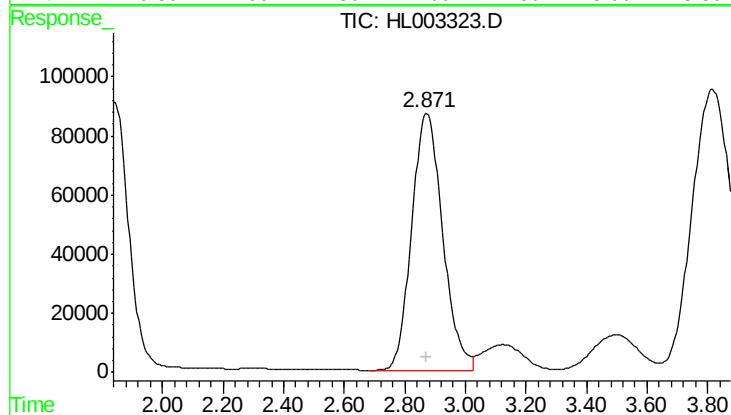

#4 1,3,5-Trinitrobenzene


R.T.: 2.873 min
Delta R.T.: 0.002 min
Response: 6170308
Conc: 505.49 ug/L

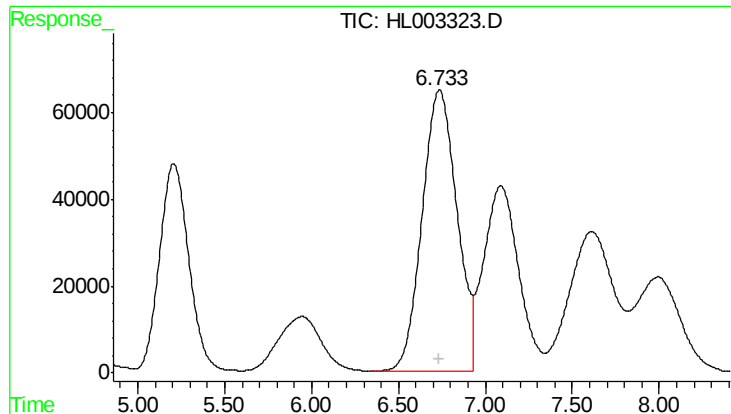

#5 Tetryl


R.T.: 6.735 min
Delta R.T.: 0.002 min
Response: 9075916
Conc: 1017.97 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

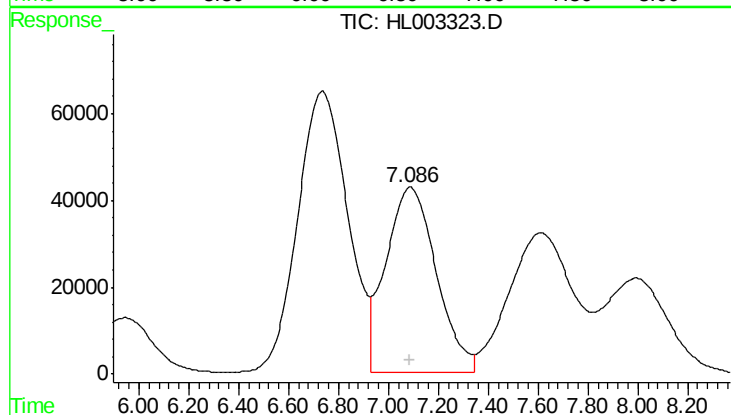


#6 2,4,6-Trinitrotoluene

R.T.: 7.089 min
Delta R.T.: 0.002 min
Response: 6036103
Conc: 512.44 ug/L

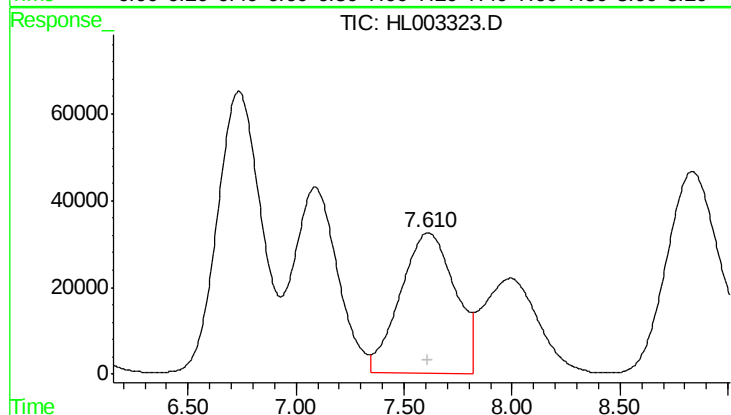


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.612 min
Delta R.T.: 0.003 min
Response: 5707788
Conc: 511.09 ug/L

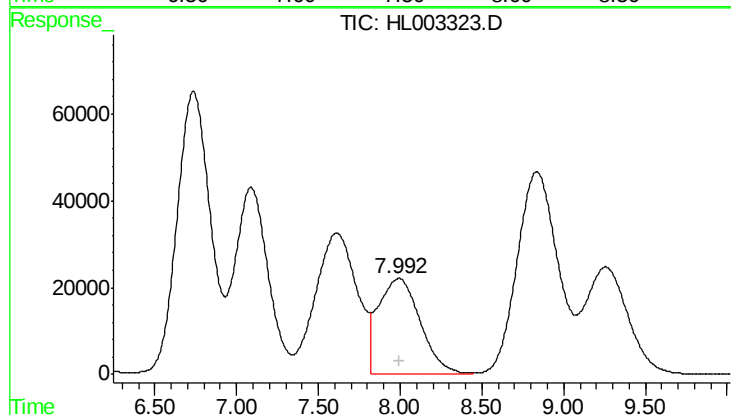

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 3906201
Conc: 517.60 ug/L

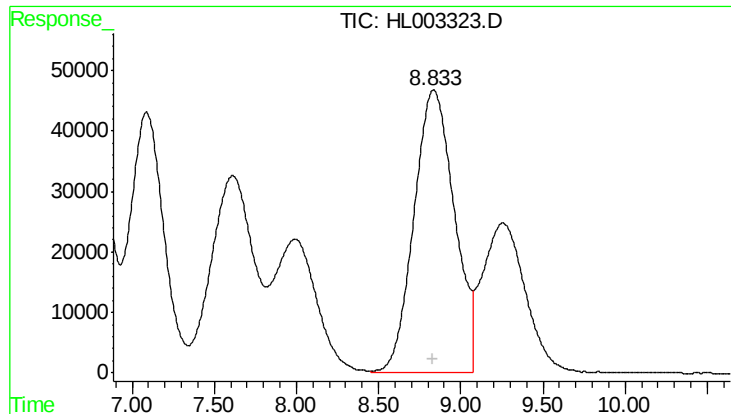

#9 2,4-Dinitrotoluene


R.T.: 8.836 min
Delta R.T.: 0.002 min
Response: 8006144
Conc: 505.51 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

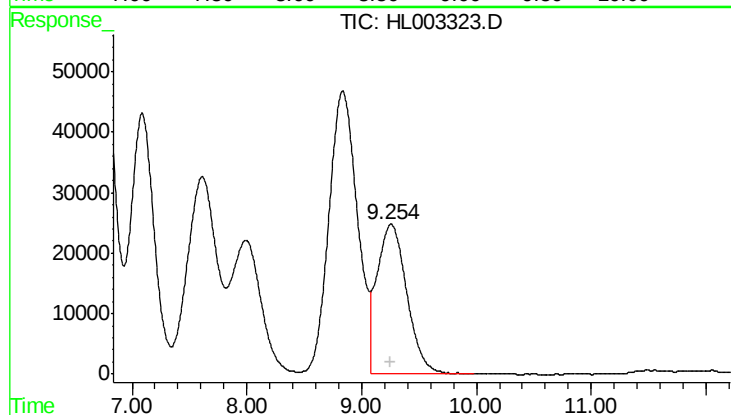


#10 2,6-Dinitrotoluene

R.T.: 9.257 min
Delta R.T.: 0.003 min
Response: 4500773
Conc: 511.33 ug/L

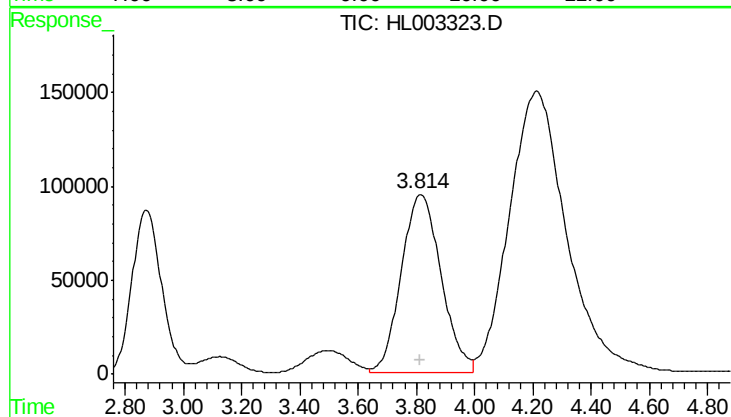


#11 1,3-Dinitrobenzene

R.T.: 3.816 min
Delta R.T.: 0.002 min
Response: 9089819
Conc: 547.40 ug/L

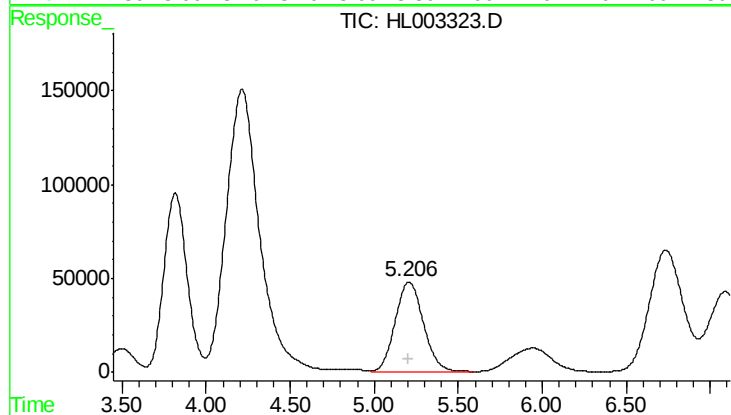

#12 Nitrobenzene


R.T.: 5.208 min
Delta R.T.: 0.002 min
Response: 5569054
Conc: 497.21 ug/L

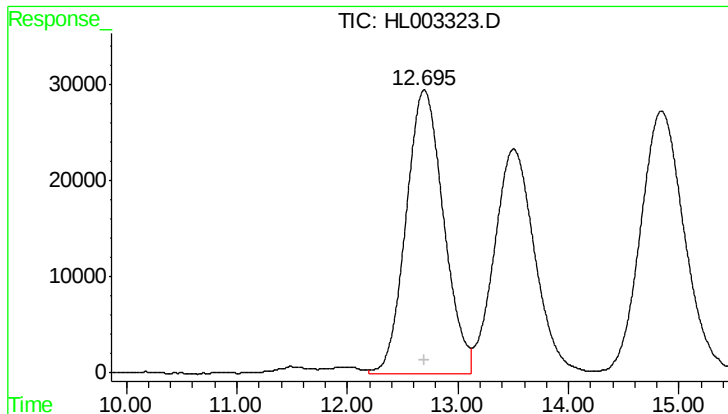

#13 2-Nitrotoluene


R.T.: 12.696 min
Delta R.T.: 0.001 min
Response: 6968167
Conc: 998.95 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

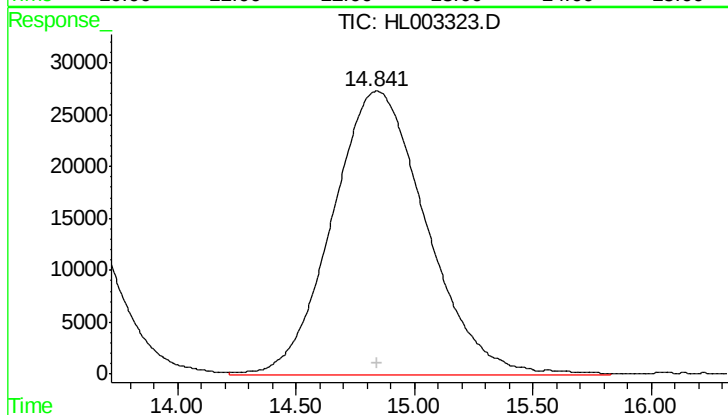


#14 3-Nitrotoluene

R.T.: 14.842 min
Delta R.T.: 0.000 min
Response: 7624209
Conc: 1032.46 ug/L

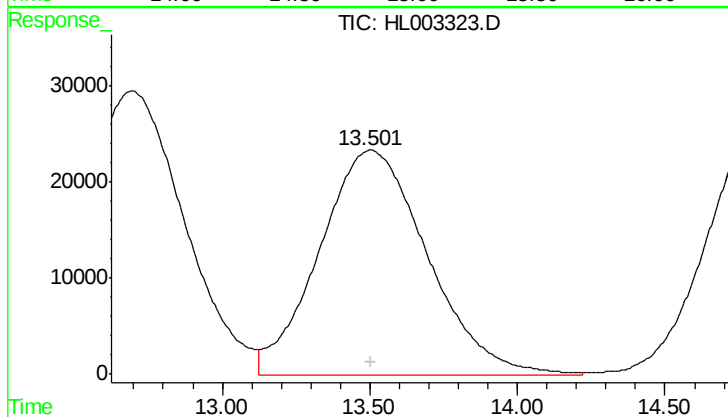


#15 4-Nitrotoluene

R.T.: 13.503 min
Delta R.T.: 0.000 min
Response: 5981370
Conc: 1005.97 ug/L

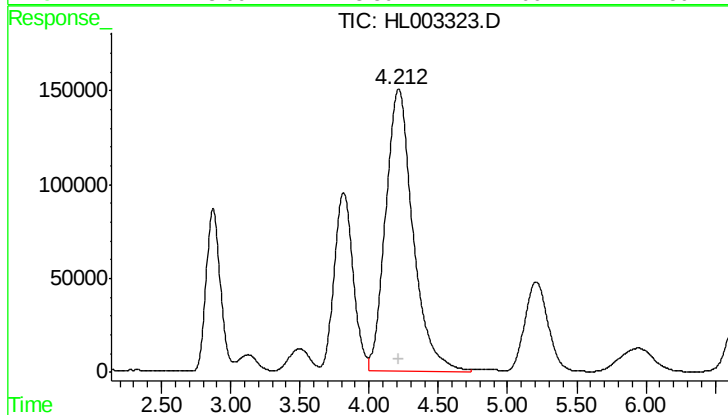

#16 3,5-Dinitroaniline

R.T.: 4.214 min
Delta R.T.: 0.002 min
Response: 20730785
Conc: 1090.08 ug/L

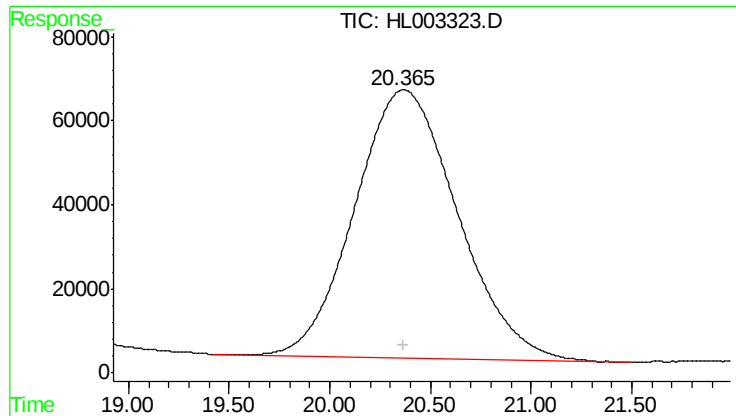

#18 PETN

R.T.: 20.367 min
Delta R.T.: 0.002 min
Response: 22748437
Conc: 2361.69 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV