



Data Path : S:\HPCHEM1\HPLC_L\Data\HL083012\
Data File : HL003417.D
Signal(s) : VWD1A.CH
Acq On : 30-Aug-2012, 14:23
Operator : HLM
Sample : 8330NG-CCV
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

Integration File: events.e
Quant Time: Sep 07 01:44:16 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL080312.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Aug 06 10:00:24 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

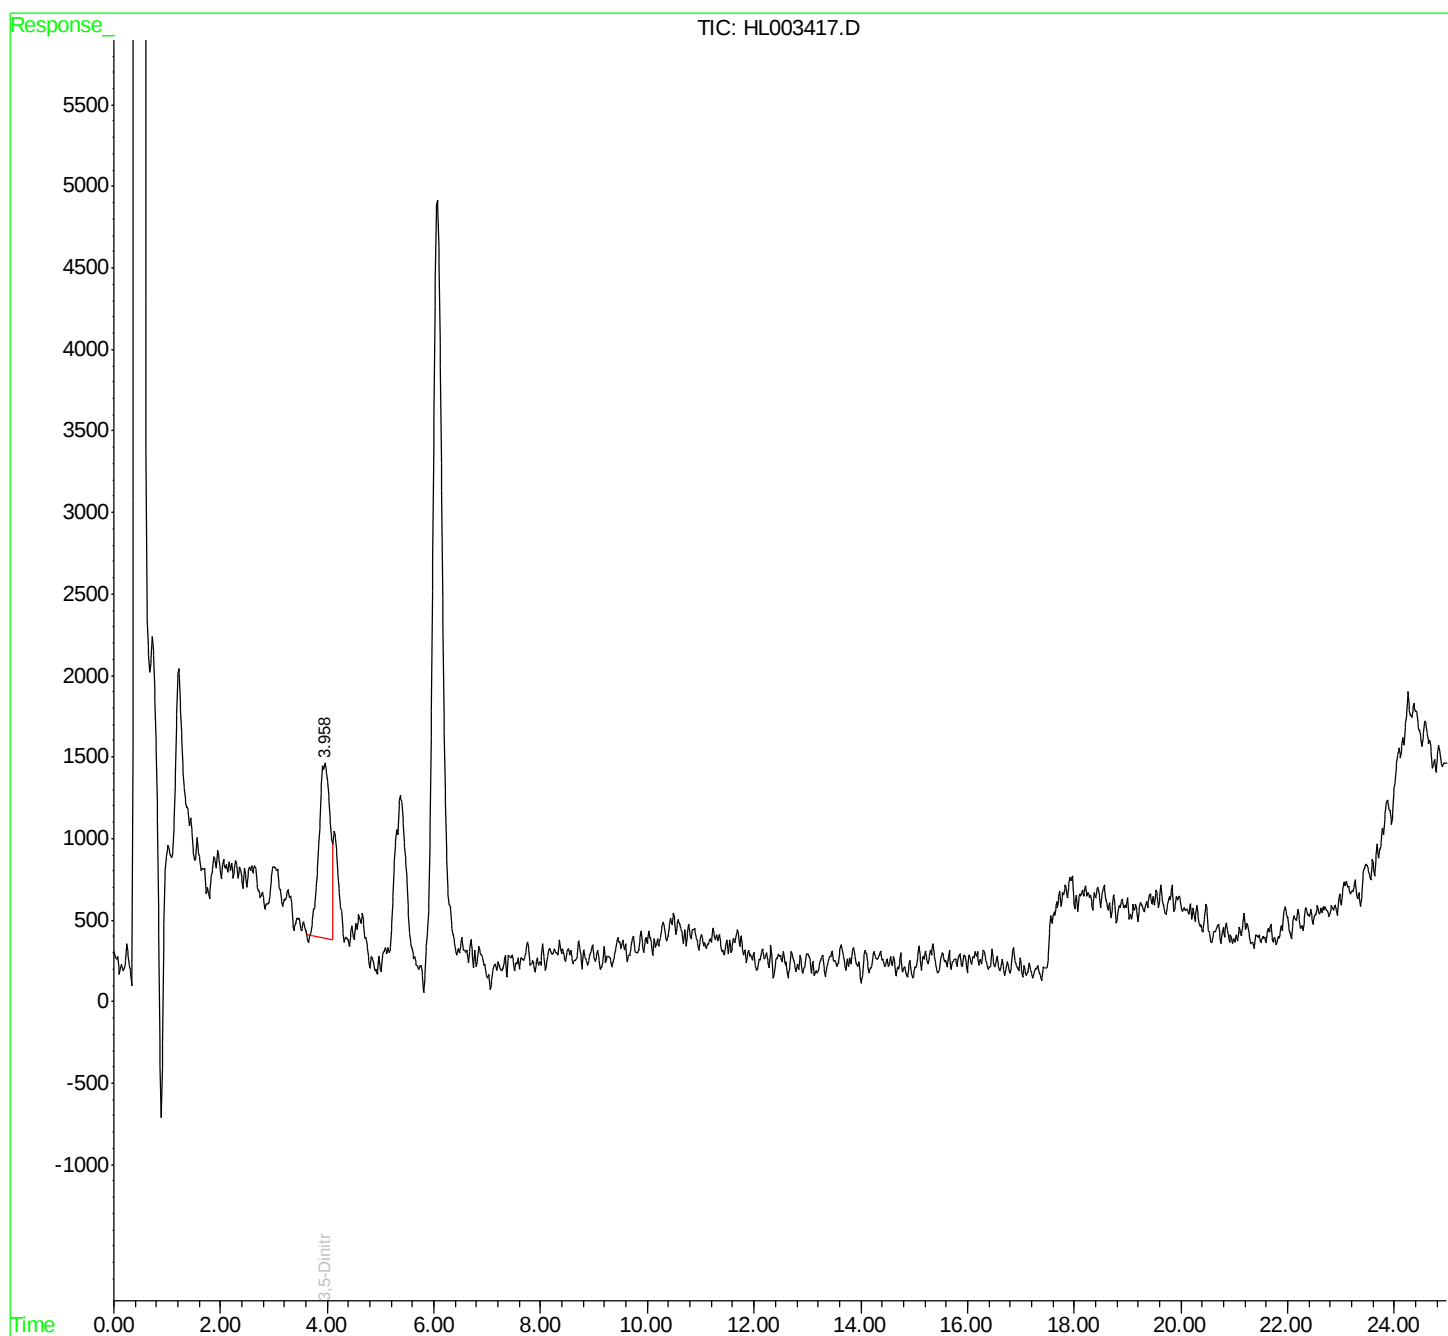


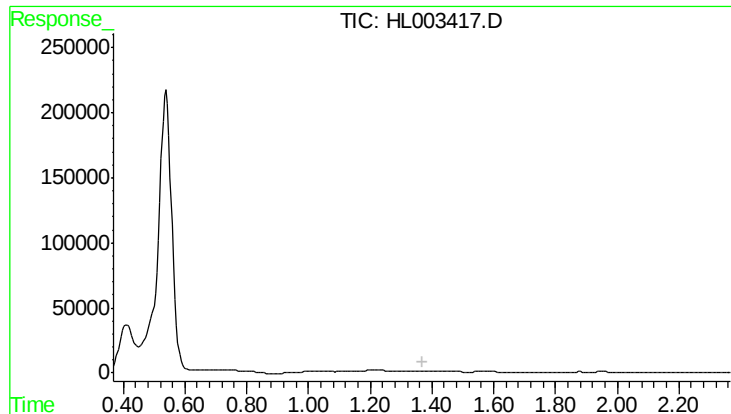

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.368 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

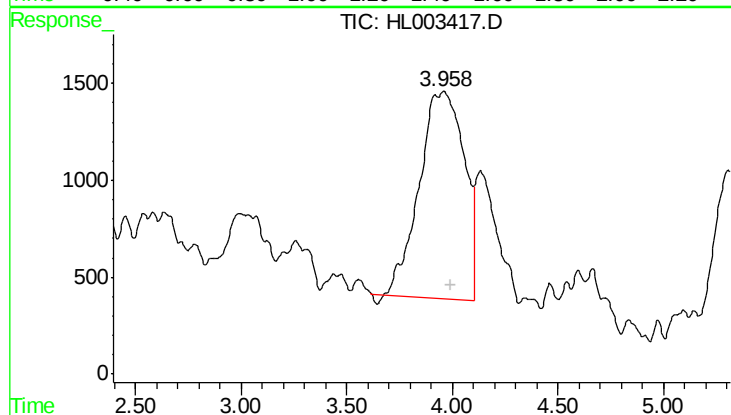

#16 3,5-Dinitroaniline

R.T.: 3.961 min
Delta R.T.: -0.031 min
Response: 156477
Conc: 11.26 ug/L

Data Path : S:\HPCHEM1\HPLC_L\Data\HL083012\
Data File : HL003417.D
Signal(s) : VWD1A.CH
Acq On : 30-Aug-2012, 14:23
Operator : HLM
Sample : 8330NG-CCV
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

Integration File: events.e
Quant Time: Sep 07 01:44:16 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL080312.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Aug 06 10:00:24 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T 3,5-Dinitroaniline	3.961f	156477	11.261 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.