

Data Path : S:\HPCHEM1\HPLC_L\Data\HL083012\
Data File : HL003422.D
Signal(s) : VWD1A.CH
Acq On : 30-Aug-2012, 16:38
Operator : HLM
Sample : PB65440BSD2
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
PB65440BSD2


Manual Integrations
APPROVED

AHPatel
9/11/2012 4:22:24 AM

Integration File: events.e
Quant Time: Sep 07 01:44:46 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL080312.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Aug 06 10:00:24 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

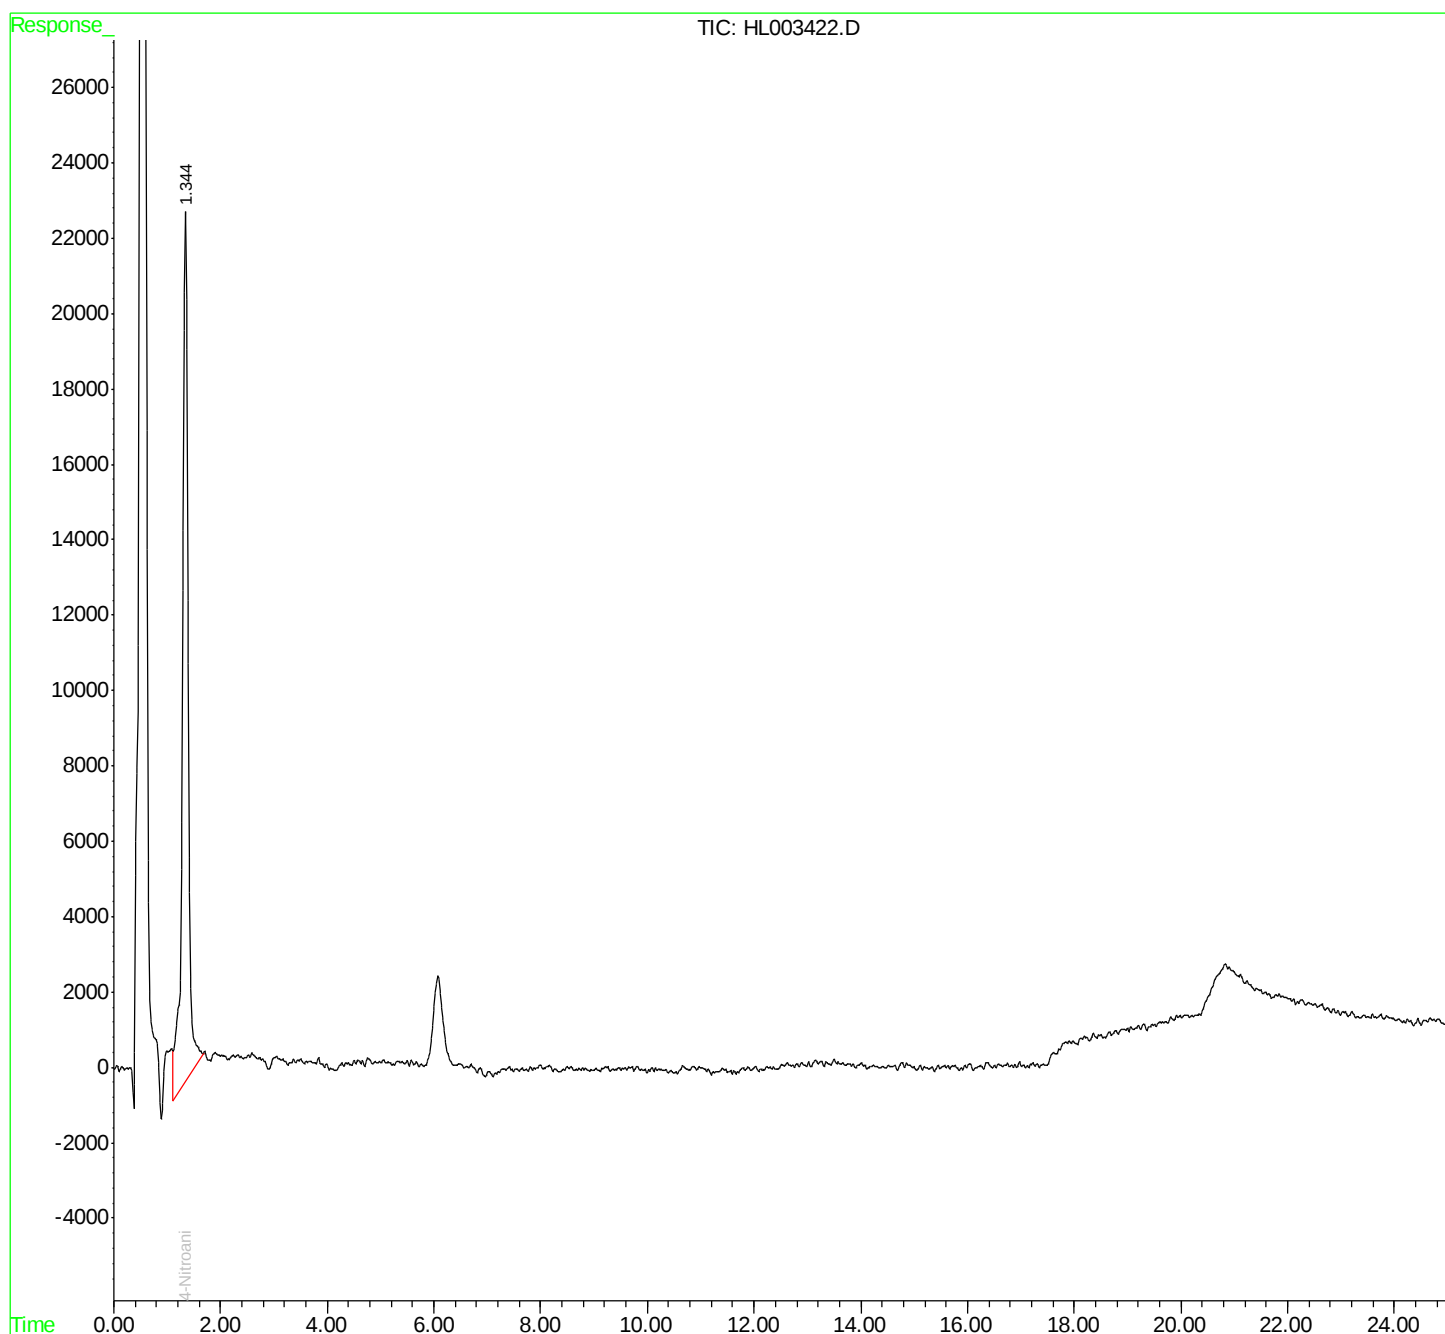

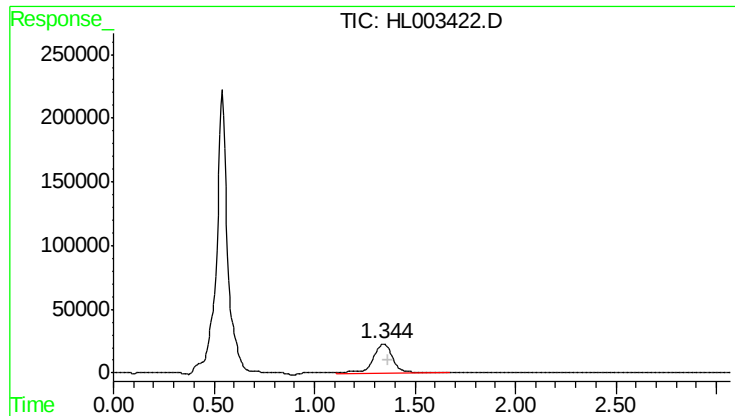

#1 4-Nitroaniline

R.T.: 1.346 min
Delta R.T.: -0.022 min
Response: 1687663
Conc: 460.15 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB65440BSD2

Manual Integrations
APPROVED

AHPatel
9/11/2012 4:22:24 AM

Data Path : S:\HPCHEM1\HPLC_L\Data\HL083012\
Data File : HL003422.D
Signal(s) : VWD1A.CH
Acq On : 30-Aug-2012, 16:38
Operator : HLM
Sample : PB65440BSD2
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
PB65440BSD2

Manual Integrations
APPROVED

AHPatel
9/11/2012 4:22:24 AM

Integration File: events.e
Quant Time: Sep 07 01:44:46 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL080312.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Mon Aug 06 10:00:24 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.346f	1687663	460.152 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 153.38%#

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.