

Data Path : S:\HPCHEM1\HPLC_L\Data\HL102412\
 Data File : HL003626.D
 Signal(s) : VWD1A.CH
 Acq On : 24-Oct-2012, 20:06
 Operator : HLM
 Sample : 8330-ICV
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL102412

Integration File: events.e
 Quant Time: Nov 16 02:31:59 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Thu Oct 25 10:56:40 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc	Units

System Monitoring Compounds				
Target Compounds				
2) T HMX	0.928	4069500	1004.887	ug/L
3) T RDX	1.790	5651515	1050.003	ug/L
4) T 1,3,5-Trinitrobenzene	2.803	12159001	1024.924	ug/L
5) T Tetryl	6.354	8922701	1047.810	ug/L
6) T 2,4,6-Trinitrotoluene	6.753	11981284	1051.473	ug/L
7) T 2-Amino-4,6-dinitroto...	7.212	11335804	1045.571	ug/L
8) T 4-Amino-2,6-dinitroto...	7.545	7609741	1054.550	ug/L
9) T 2,4-Dinitrotoluene	8.430	15142965	948.329	ug/L
10) T 2,6-Dinitrotoluene	8.819	8602217	998.070	ug/L
11) T 1,3-Dinitrobenzene	3.713	16627028	1004.922	ug/L
12) T Nitrobenzene	4.991	10670860	997.073	ug/L
13) T 2-Nitrotoluene	12.169	6883530	1016.299	ug/L
14) T 3-Nitrotoluene	14.256	7322148	1016.129	ug/L
15) T 4-Nitrotoluene	12.953	5781488	994.144	ug/L
16) T 3,5-Dinitroaniline	4.049	14152666	901.380	ug/L
18) T PETN	19.433	8785184	948.648	ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL102412\
Data File : HL003626.D
Signal(s) : VWD1A.CH
Acq On : 24-Oct-2012, 20:06
Operator : HLM
Sample : 8330-ICV
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412

Integration File: events.e
Quant Time: Nov 16 02:31:59 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

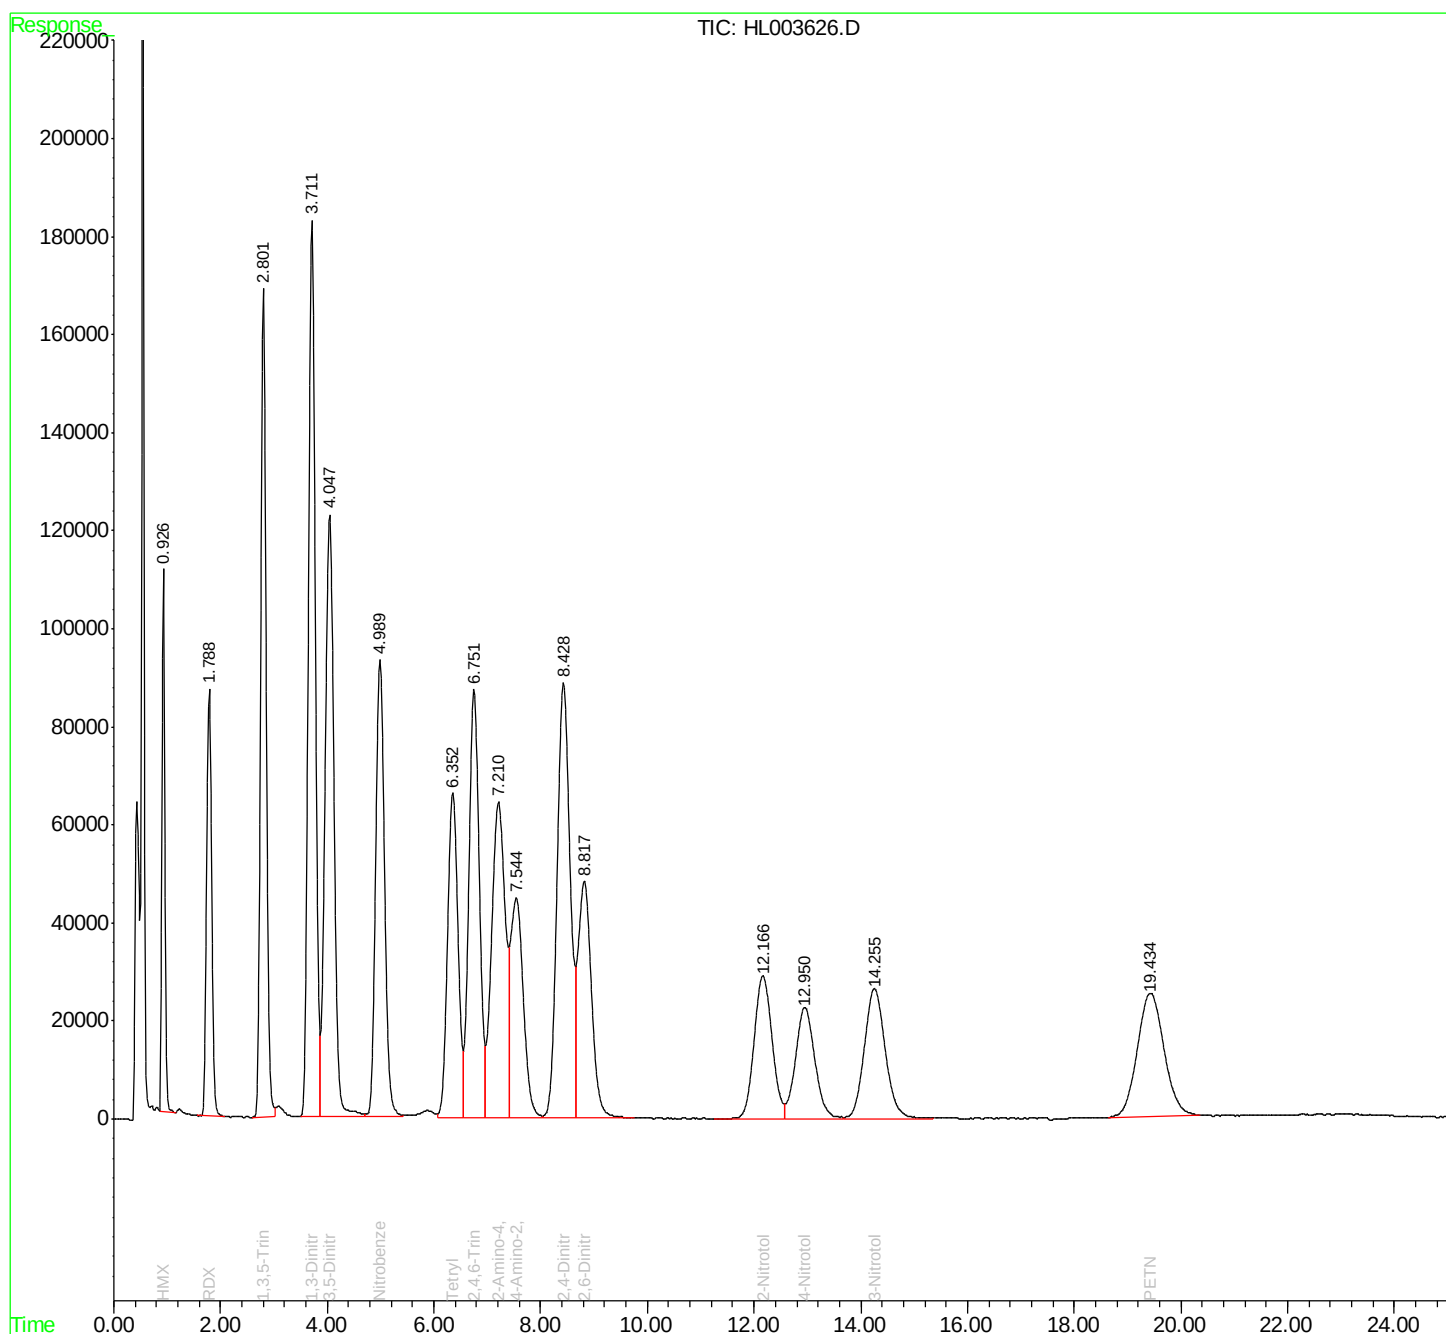


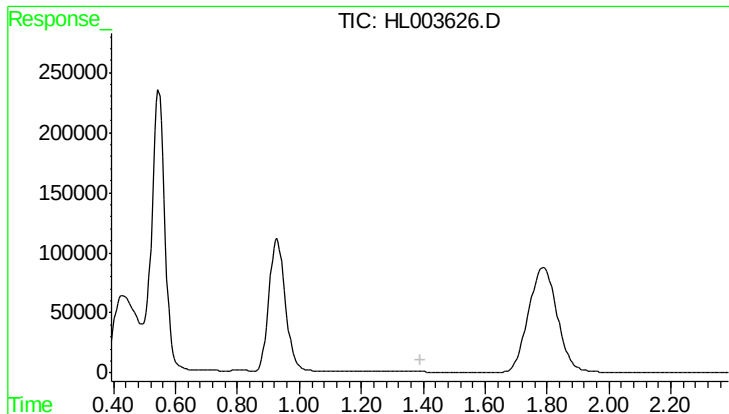

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.391 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412

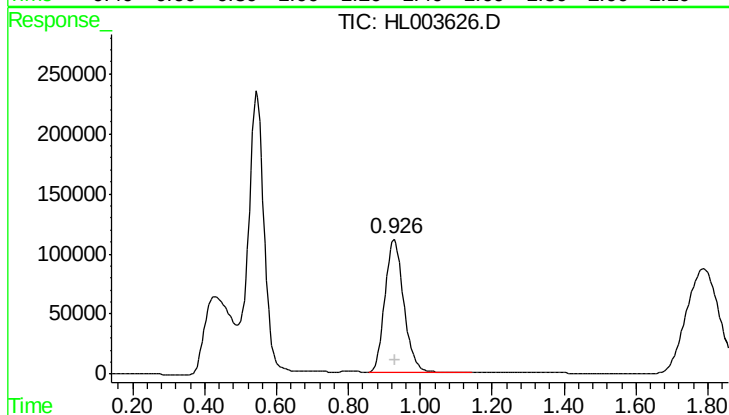


#2 HMX

R.T.: 0.928 min
Delta R.T.: -0.002 min
Response: 4069500
Conc: 1004.89 ug/L

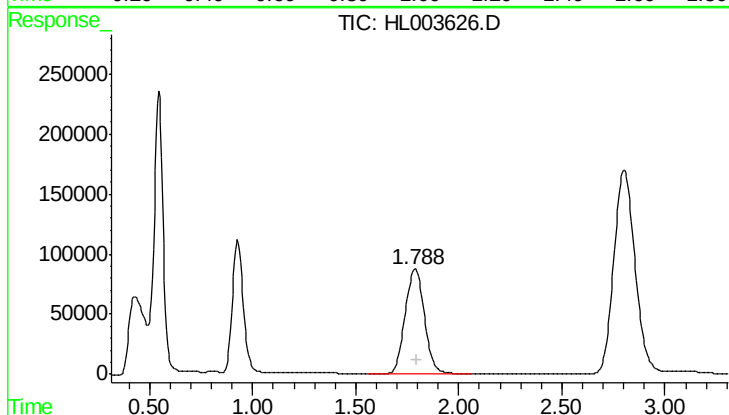


#3 RDX

R.T.: 1.790 min
Delta R.T.: -0.003 min
Response: 5651515
Conc: 1050.00 ug/L

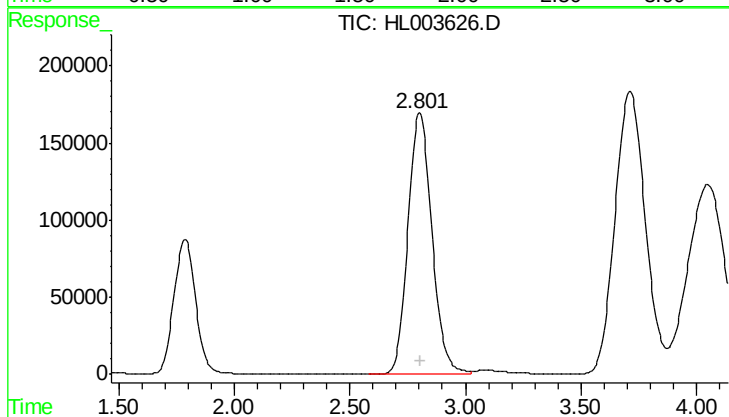

#4 1,3,5-Trinitrobenzene


R.T.: 2.803 min
Delta R.T.: -0.004 min
Response: 12159001
Conc: 1024.92 ug/L

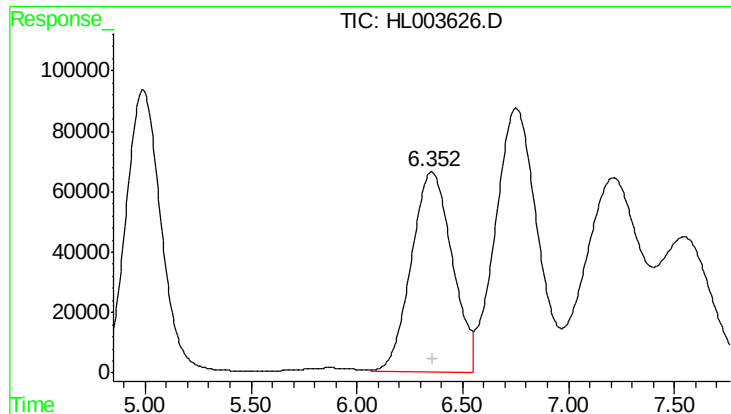

#5 Tetryl


R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 8922701
Conc: 1047.81 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412

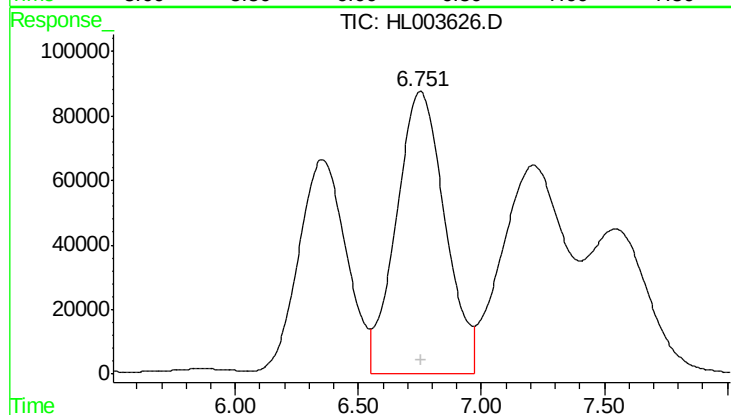


#6 2,4,6-Trinitrotoluene

R.T.: 6.753 min
Delta R.T.: -0.004 min
Response: 11981284
Conc: 1051.47 ug/L

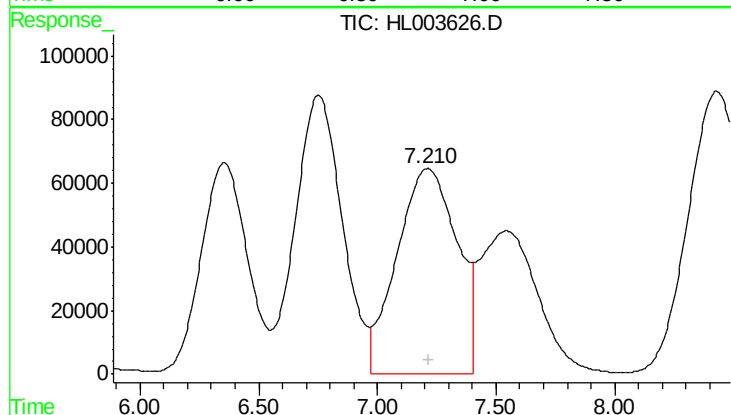


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.212 min
Delta R.T.: -0.003 min
Response: 11335804
Conc: 1045.57 ug/L

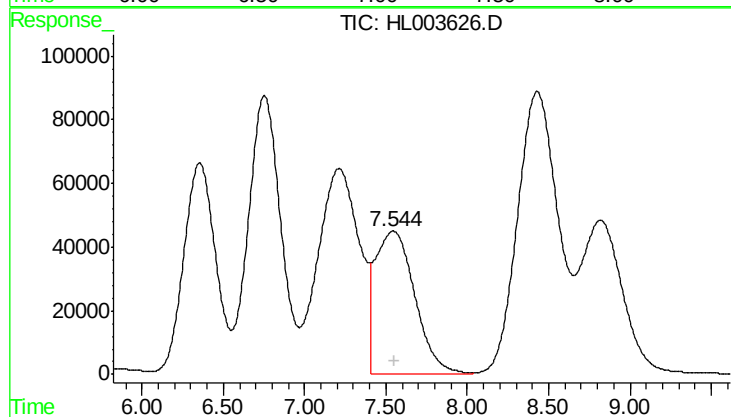

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.545 min
Delta R.T.: -0.003 min
Response: 7609741
Conc: 1054.55 ug/L

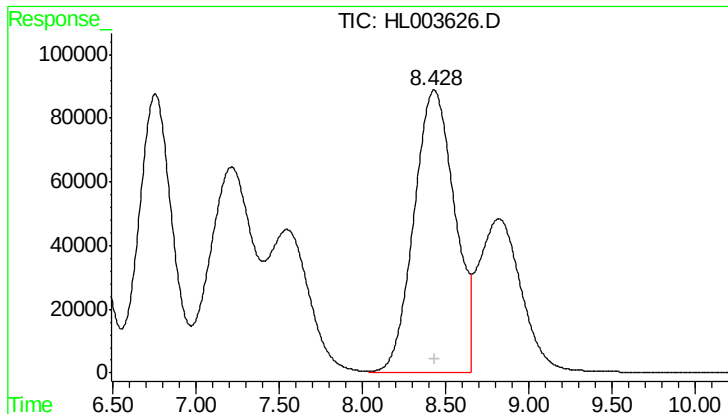

#9 2,4-Dinitrotoluene


R.T.: 8.430 min
Delta R.T.: -0.005 min
Response: 15142965
Conc: 948.33 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412

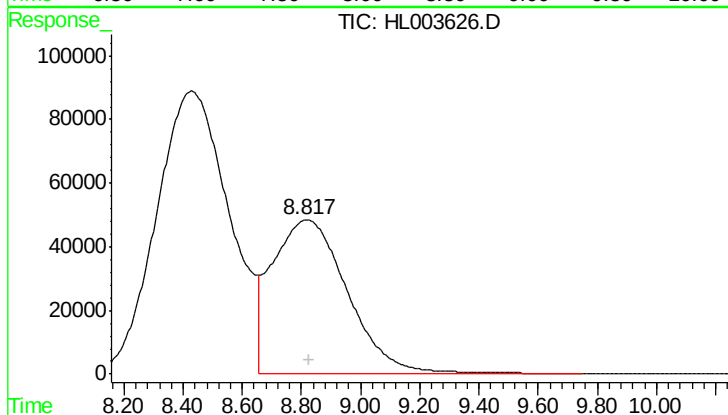


#10 2,6-Dinitrotoluene

R.T.: 8.819 min
Delta R.T.: -0.005 min
Response: 8602217
Conc: 998.07 ug/L

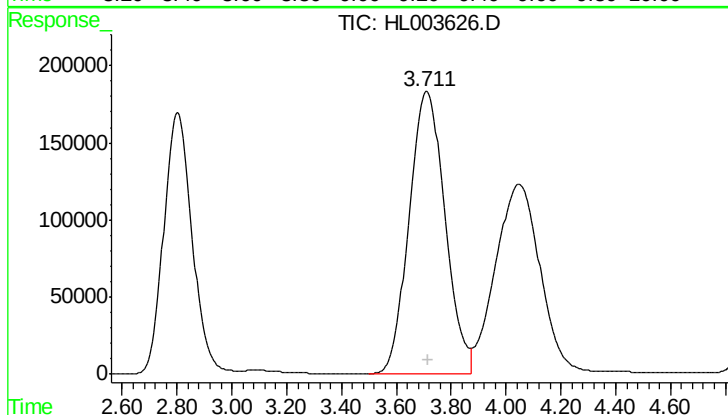


#11 1,3-Dinitrobenzene

R.T.: 3.713 min
Delta R.T.: -0.004 min
Response: 16627028
Conc: 1004.92 ug/L

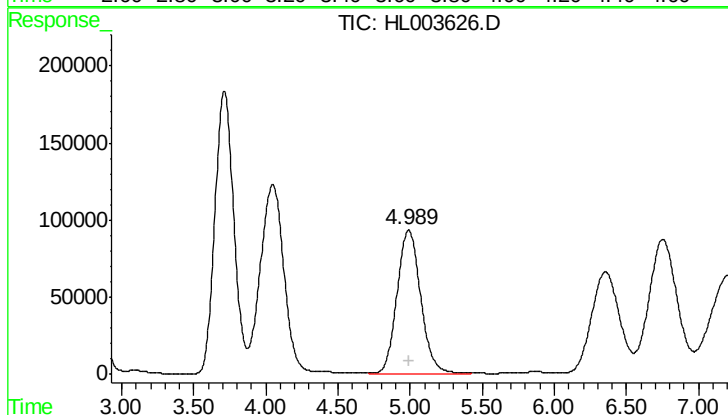

#12 Nitrobenzene


R.T.: 4.991 min
Delta R.T.: -0.005 min
Response: 10670860
Conc: 997.07 ug/L

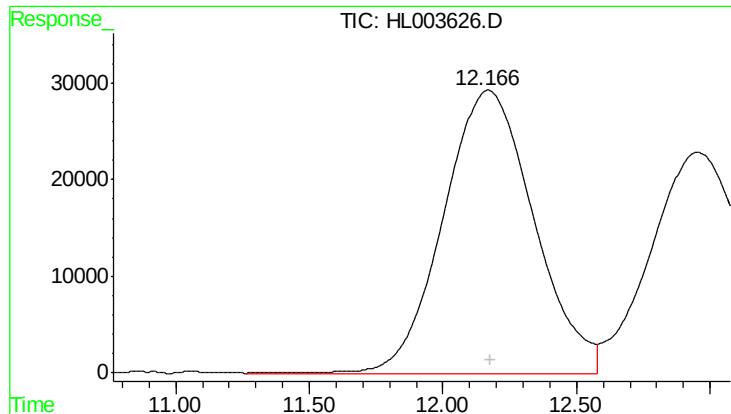

#13 2-Nitrotoluene


R.T.: 12.169 min
Delta R.T.: -0.007 min
Response: 6883530
Conc: 1016.30 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412

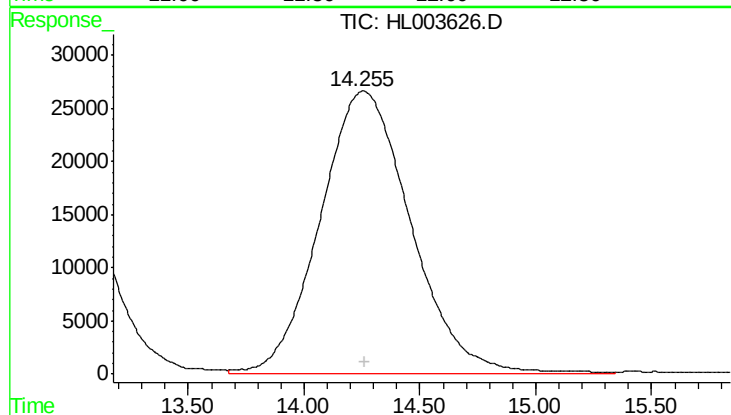


#14 3-Nitrotoluene

R.T.: 14.256 min
Delta R.T.: -0.008 min
Response: 7322148
Conc: 1016.13 ug/L

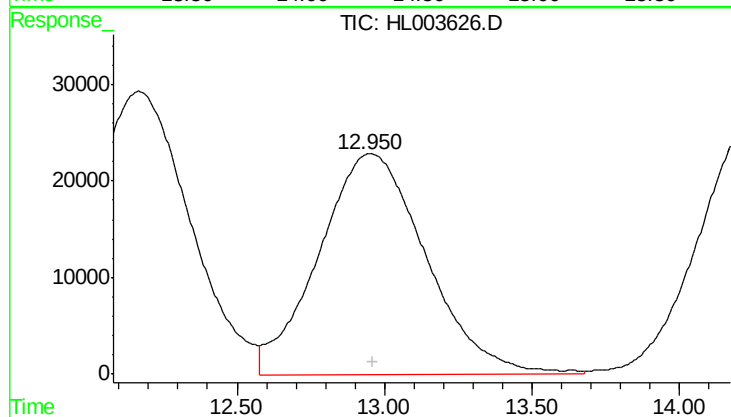


#15 4-Nitrotoluene

R.T.: 12.953 min
Delta R.T.: -0.008 min
Response: 5781488
Conc: 994.14 ug/L

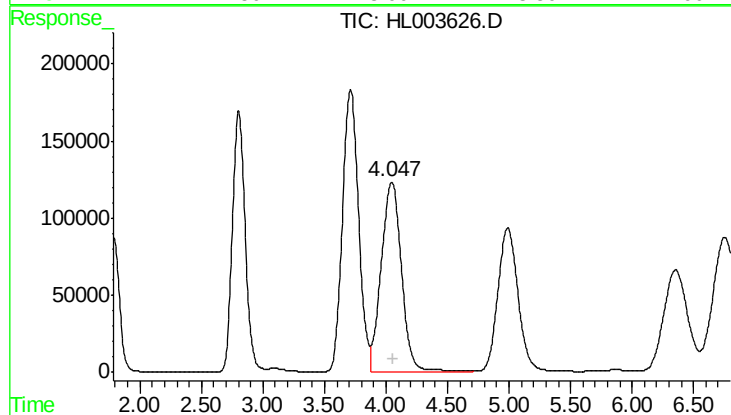

#16 3,5-Dinitroaniline

R.T.: 4.049 min
Delta R.T.: -0.006 min
Response: 14152666
Conc: 901.38 ug/L

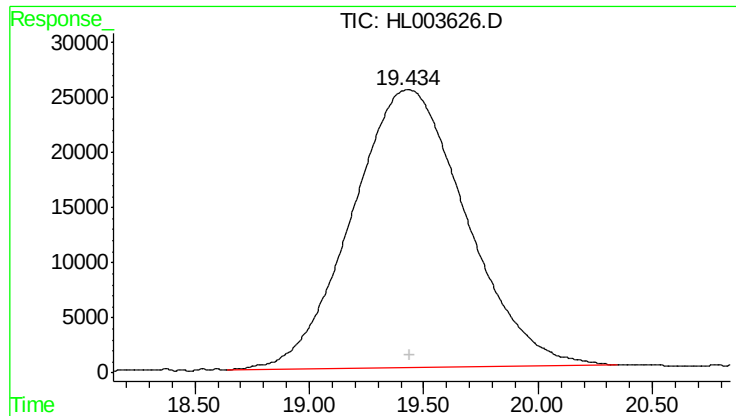

#18 PETN

R.T.: 19.433 min
Delta R.T.: -0.006 min
Response: 8785184
Conc: 948.65 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL102412